


Dynamic μ Scanbody




The Micro-Scan System from Dynamic Abutment® Solutions comprises the latest technology developed by our Research & Development department to provide top precision and accuracy in the scanning and milling process, incorporating the angled system. We certify a minimum precision of $\pm 3 \mu\text{m}$

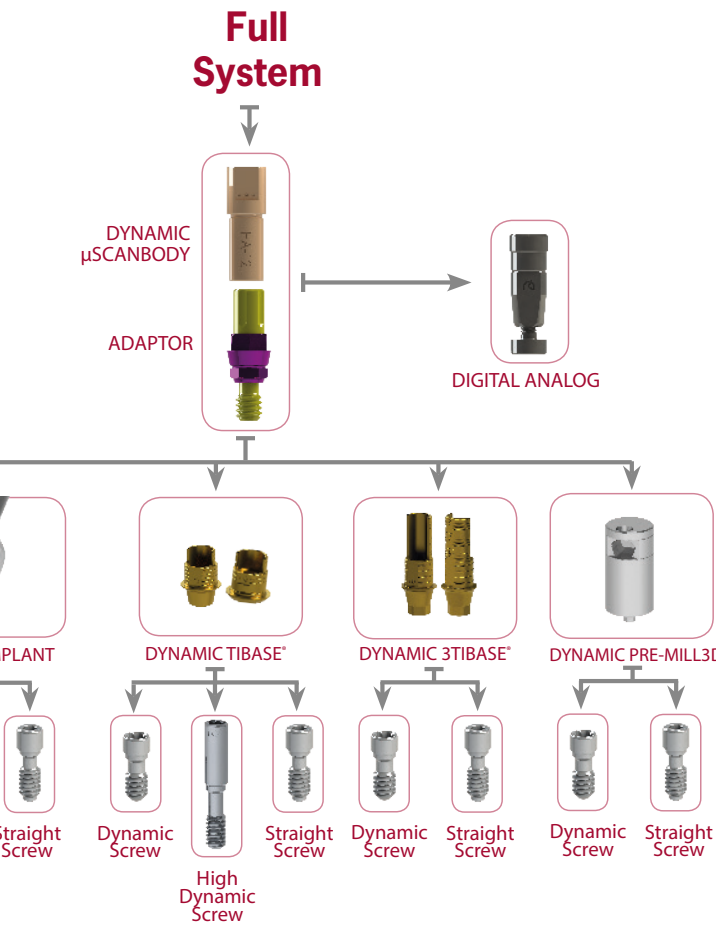

AV. BLONDEL, 54 3º
25002 LLEIDA (SPAIN)
TEL. +34 873 450 709
das@dynamicabutment.com
www.dynamicabutment.com



DYNAMIC μ SCANBODY

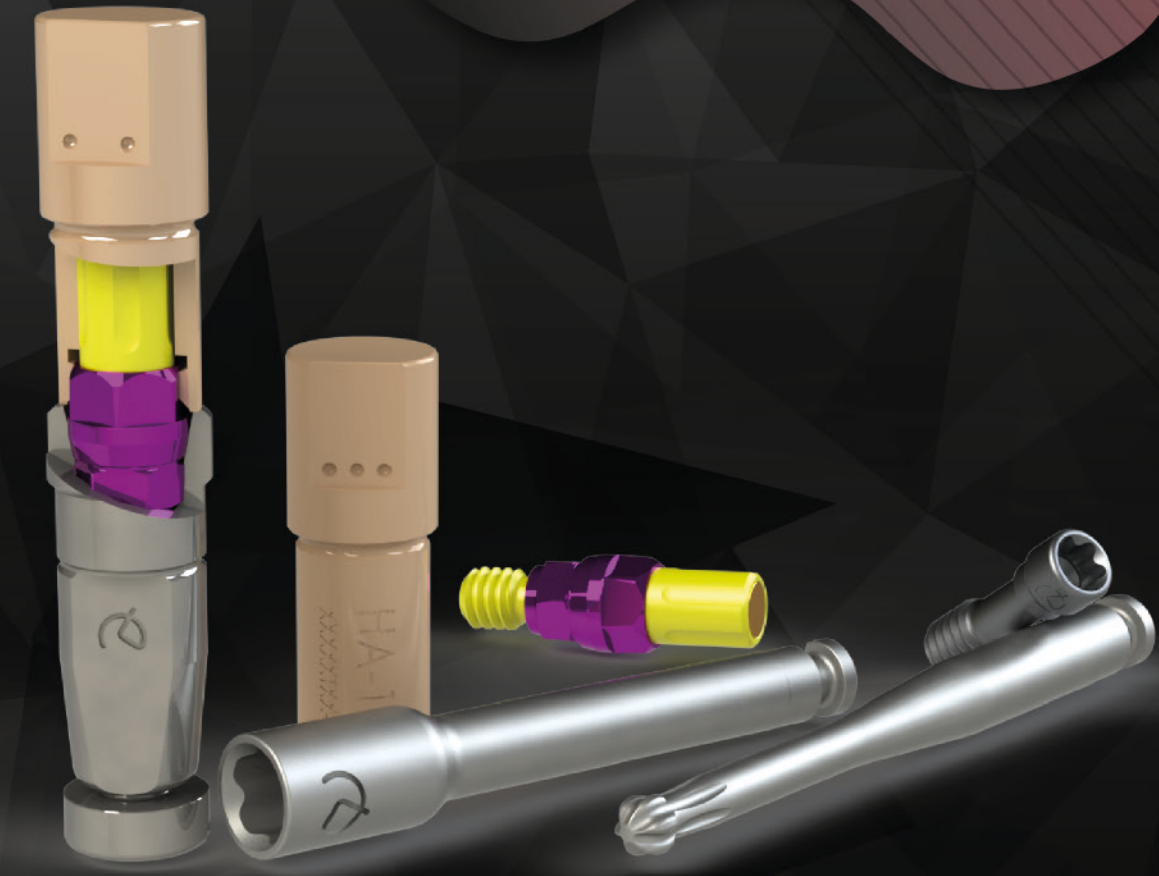

VERSION 2019-01



Dynamic μ Scanbody

Compatibilities available





Hole free scanbody and not screwed

The scanbody is not screwed into the implant, so there are no holes in the upper section which means the Z axis is free to improve scanbody scanning.




3 heights (8mm, 10mm, 12mm)

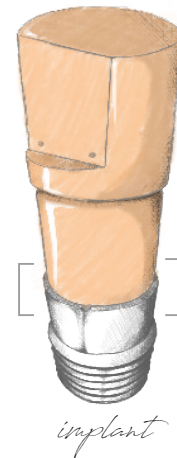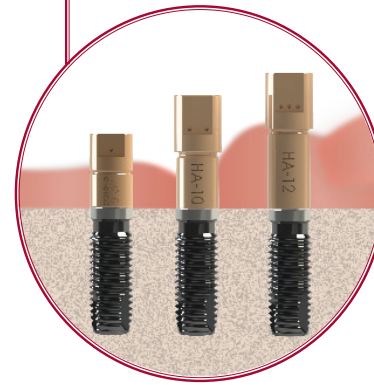

The diameter of the scanbody is always equal or smaller than the implant diameter.




1 adaptor for 3 scanbodies of different heights

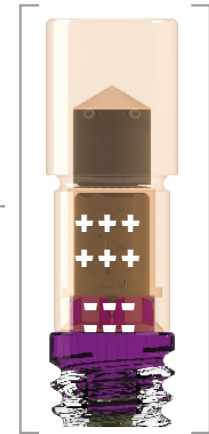

Scanbody and adaptor fastened using a **MAGNET**

Special screwdriver for adaptors.




Enables to know the position of the implant faces
Screwed into the implant

Digital Analog



3D Printed Model


Digital analog of the dental implant to simulate implant position in a 3D printed dental model.

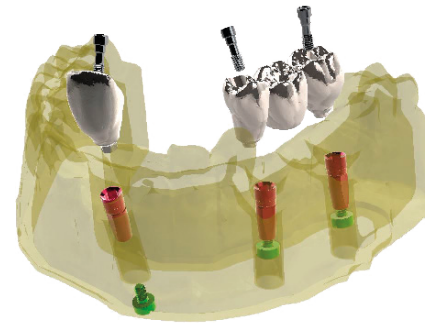


Using libraries you can design the dental model where digital analogues will be inserted.




Concave notch
Top precision in longitudinal position




Curved Surface
Accuracy of orientation guaranteed



Longitudinal cut
Longitudinal cut to avoid rotation X-Y



Screwed fastening
Prevents the analog from moving in Z

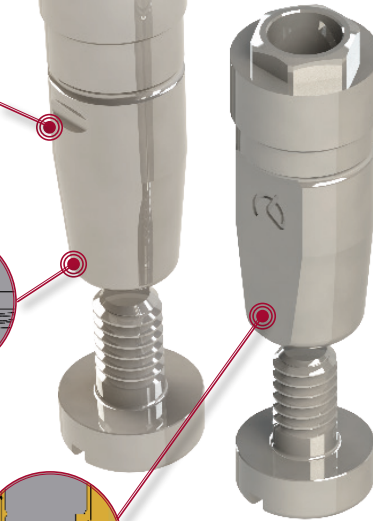

For over 500 compatibilities

CODE	MAIN CONNECTION*	SCANBODY	REFERENCE		
0002	Biomet 3i Certain RP	HA	52.410.101.01-2		
0007	Astra Evolution 4,2				
0017	MIS C1 RP				
0022	Nobel Biocare Active RP				
0024	Nobel Biocare Branemark RP				
0030	Osstem Implant TS RP				
0040	Zimmer NP Screw-Vent 3,5				
0057	Biomet 3i Certain WP				
0064	S&M Outlink 4,1				
0005	Astra Lilac			HB	52.410.102.01-2
0018	MIS C1 WP				
0041	Zimmer Screw-Vent 4,5				
0052	Bego S/RI 4,5				
0091	Astra Evolution 4,8				
0001	Biomet 3i Certain NP	HC	52.410.103.01-2		
0004	Astra Aqua				
0021	Nobel Biocare Active NP				
0023	Nobel Biocare Branemark NP				
0029	Osstem Implant TS Mini				
0038	Xive S 3,4				
0083	Klockner Vega RV				
0003	Biomet 3i Osseotite NP			HD	52.410.104.01-2
0015	Megagen AnyRidge RP				
0006	Astra Evolution 3,6			HE	52.410.105.01-2
0019	MIS M4 NP				
0044	Keystone Prima NP				
0075	Ankylos				
0082	Klockner Vega NV				
0008	Astra Evolution Uni-Abutment	HF	52.408.113.01-2		
0009	BTI External NP	HG	52.410.114.01-2		
0039	Xive S 3,8	HH	52.410.116.01-2		
0049	Bego RS/RXS 3				
0050	Bego S/RI 3,25-3,75	HI	52.410.117.01-2		
0085	Xive S 4,5				
0125	Medentis ICX-Templant 4,1			HJ	52.410.118.01-2
0051	Bego S/RI 4,1				
0045	Keystone Prima RP				
0058	Biomet 3i Osseotite WP	HK	52.410.120.01-2		
0032	S&M Premium Khono 3,80				

CODE	MAIN CONNECTION*	SCANBODY	REFERENCE
0065	S&M Premium Khono 4,25	HL	52.410.121.01-2
0060	BTI External WP	HM	52.410.122.01-2
0047	Neoss 3,4	HN	52.409.123.01-2
0048	Neoss 4,1		
0151	BTI Multi-IM Universal	HO	52.410.124.01-2
0080	Zimmer Screw-Vent 5,7		
0046	Keystone Prima WP	HP	52.410.125.01-2
0061	Nobel Biocare Branemark WP		
0124	Nobel Biocare Active WP		
0081	Bego S/RI 5,5	HR	52.410.126.01-2
0090	Astra Evolution 3,0	HS	52.401.128.01-2
0109	Astra Yellow		
0136	Alphabio Conical Hex. Connection		
0159	Nobel Biocare Active 3,0		
0164	Biotech Dental Kontakt XNP	HT	52.410.129.01-2
0092	Astra Evolution 5,4		
0025	Nobel Biocare Multi Unit RP	MA	52.410.111.01-2
0020	MIS Multi Unit St	MB	52.408.112.01-2
0025	Nobel Biocare Multi Unit RP		
0163	Anthogyr Multi-Unit 4,8	OA	52.410.110.01-2
0037	Straumann Internal Octagon 4,8		
0074	Straumann Synocta 4,8		
0096	Straumann Internal Octagon 6,5	OB	52.410.119.01-2
0054	Klockner Essential Cone 4,5		
0016	MIS C1 NP	SA	52.410.106.01-2
0033	Straumann Bone Level NP		
0035	Straumann Bone Level RP	SB	52.410.107.01-2
0010	BTI Internal RP	SC	52.410.115.01-2
0160	Straumann Tissue Level NNC	SD	52.410.131.01-2
0011	Camlog Screw-Line 3,8	TA	52.410.108.01-2
0026	Nobel Biocare Replace 3,5		
0012	Camlog Screw-Line 4,3	TB	52.410.109.01-2
0027	Nobel Biocare Replace 4,3		
0028	Nobel Biocare Replace 5,0	TC	52.410.130.01-2
0129	Nobel Biocare Replace 6,0		
0149	Anthogyr Axiom REG/PX XNP	TD	52.410.132.01-2
0162	Anthogyr Axiom REG/PX WP		
0161	Anthogyr Axiom REG/PX RP		
0165	Biotech Dental Kontakt RP		

* Check new compatibilities available emailing: das@dynamicabutment.com

Connecting element between the scanbody and the implant/analog. Marked with different colors according to compatibility.

*See CAD-CAM Solutions catalogue