



# DIGITAL SOLUTIONS PRODUCT REFERENCES

CATALOGUE

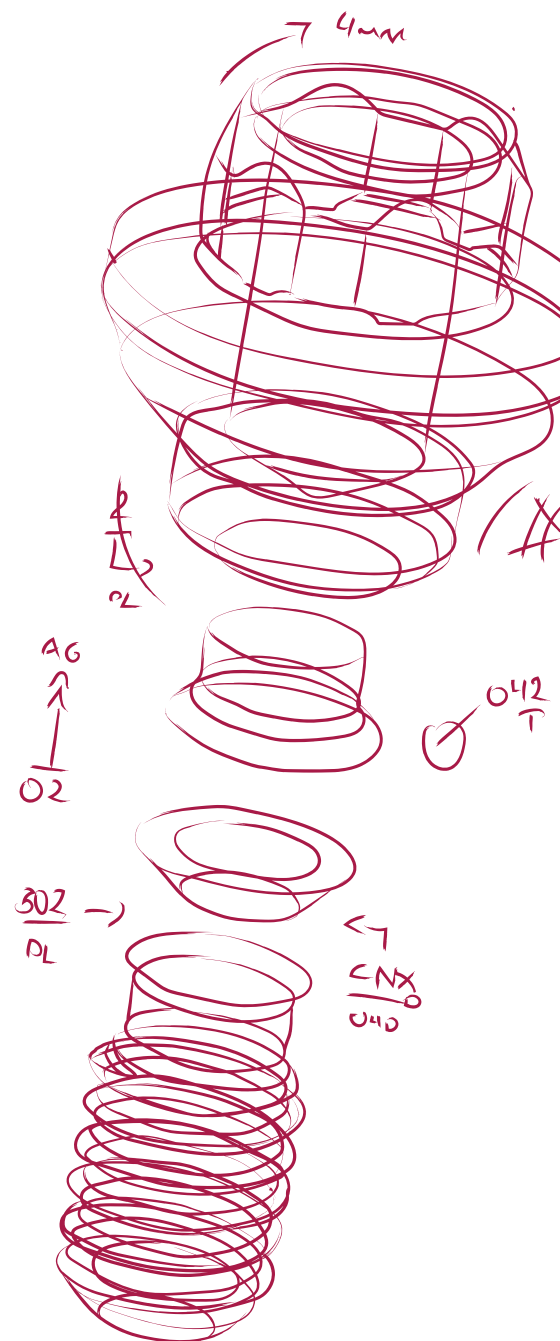

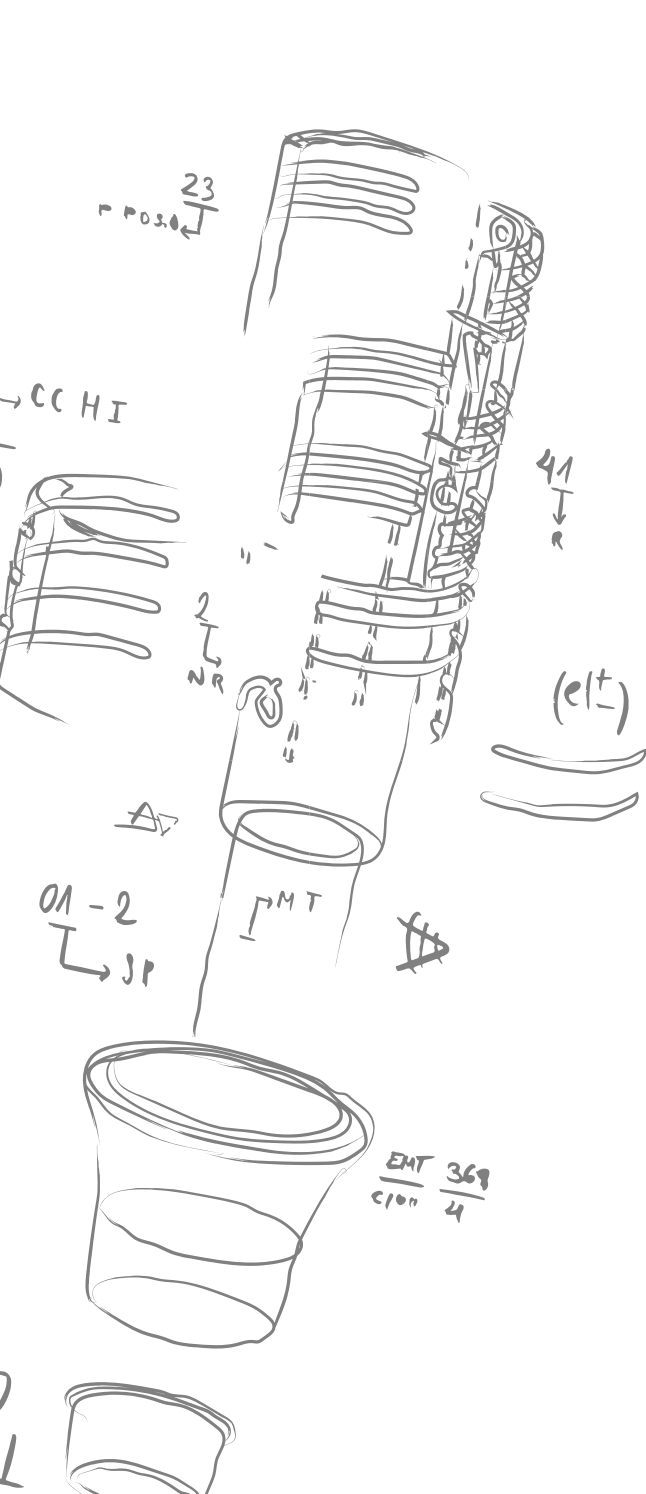

## DYNAMIC ABUTMENT SOLUTIONS

---

Virginia Woolf, 17  
25005 · Lleida (Spain)

INTERNATIONAL +34 873 450 709  
das@dynamicabutment.com

SPAIN +34 973 289 580  
spain@dynamicabutment.com



Dynamic Abutment Solutions is the trademark of the manufacturer Talladium España S.L. The information included in this catalogue is exclusively addressed to professionals in dental sector.

All commercial trademarks mentioned herein are fully registered by their respective companies, and the images that appear are just to provide an orientation. Talladium reserves the right to modify this document without previous notice. Talladium is not responsible for the inadequate execution of these products if the warning indications corresponding to every reference are not contemplated.

Ask about the products available with CE legislation. Some of the products are not authorized for sale and distribution or do not have a sales license in some countries according to other legislations. Information: [das@dynamicabutment.com](mailto:das@dynamicabutment.com).

# INDEX

<b>LIST OF COMPATIBILITIES AVAILABLE</b>	<b>5</b>
<b>COMPATIBILITIES AVAILABLE</b>	<b>9</b>
<b>COMPATIBILITIES AND REFERENCES</b>	<b>43</b>
<b>DAS LIBRARIES</b>	<b>332</b>
<b>MULTI-UNIT DAS LIBRARIES</b>	<b>333</b>
<b>DYNAMIC SCREWS TECHNICAL SPECIFICATIONS</b>	<b>334</b>
<b>STRAIGHT SCREWS TECHNICAL SPECIFICATIONS</b>	<b>336</b>
<b>SCREWDRIVERS AND STRAIGHT SCREWS</b>	<b>337</b>
<b>DYNAMIC MILLING TOOL SPECIFICATIONS</b>	<b>338</b>
<b>SCREWDRIVERS AND COMPLEMENTS</b>	<b>340</b>
<b>DAS MU SYSTEM COMPONENTS</b>	<b>341</b>
<b>INTERNAL DAS MU SYSTEM COMPONENTS</b>	<b>343</b>



## LIST OF COMPATIBILITIES AVAILABLE



AB	CONEXÃO SISTEMA DE PRÓTESE	HAHN IMPLANT (GLIDEWELL)	NEOBIOTECH	SIN IMPLANTS
ACE			NEODENT	
ADIN	CORTEX	HIOSSSEN	NEOSS	SOUTHERN IMPLANTS
ALFA-GATE	C-TECH	HI-TEC		
ALPHABIO	COWELLMEDI	IBS	NOBEL BIOCARE	STERI-OSS
ALPHA-DENT	DENTAL TECH	IDO IMPLANTS	NORIS MEDICAL	STERNGOLD
ANCLADEN	DENTAURUM	IHDE DENTAL (IMBIODENT)	NORMON	STRAUMANN
ANKYLOS	DENTEGRIS	IMPLANT DIRECT	NOVA IMPLANTS	SURCAM DENTAL
ANTHOGYR	DENTEM			SYBRON IMPLANT SOLUTIONS
ARDS	DENTIS	IMPLANT GENESIS	OSSTEM IMPLANT	SYSTHEX
ASTRA	DENTIUM	IMPLANTSWISS	OSTEOPLUS	TBR
AVINENT	DIO IMPLANTS	INTRA-LOCK	OXY	TITANIUM-FIX
B&W		JDENTALCARE	PALTOP	TREE-OSS
BEGO	DITRON	KEYSTONE	P-I BRANEMARK	TRI DENTAL IMPLANTS
BIOCONCEPT	DMI DENTAL SUPPLY	KLOCKNER	PHIBO	TRINON
BIOGENESIS	DSP BIOMEDICAL	KUWOTECH	POINT IMPLANT	UFIT
BIOHORIZONS	EASY IMPLANT	LASAK		
BIOMET 3i	ECKERMANN	LEADER	PROCLINIC	VULKAN IMPLANTS
BIOLOK	ELITE MEDICA	MEDENTIKA	PROTEG IMPLANTS	WARANTEC (ONEPLANT)
BIONER	EUROTEKNIKA	MEDENTIS	RADHEX	WIN
BIOTEC	F&B IMPLANT (FIT & BRILLIANT)	MEGAGEN	REFLECT	XIVE
BIOTEM		MICRODENT	RITTER	YES IMPLANT
BREDDENT MEDICAL	GALIMPLANT	MIS	ROOTT	YOUSE IMPLANTS
BTI	GC TECH	MONOIMPLANT	SEWON MEDIX	ZIACOM
BTK	GMI (ILERIMPLANT)	MOZO-GRAU (TICARE)	SIC INVENT	ZIMMER
CAMLOG	GT MEDICAL	MPI	SIGNO VINCES	

**MULTI-UNIT**  
DAS SYSTEM

**DYNAMIC**  
DAS SYSTEM

## COMPATIBILITIES AVAILABLE



AB	MODEL	IMPLANT	PLATFORM	CODE	
	I2	3,5/3,75/4,2/4,5/	STANDARD	0040	131
		5/6	STANDARD	0040	131
	I22	3,75/4,22	STANDARD	0040	131
	I5	3,5/3,75/4,2/4,5/	STANDARD	0040	131
		5/6/7/8	STANDARD	0040	131
	I55	3,75/4,2/4,5	STANDARD	0040	131
		5/6/7/8	STANDARD	0040	131
	I10	4,2/5	STANDARD	0040	131
	I15	6/7/8	STANDARD	0040	131
	MULTI UNIT D1-P64	Multi Unit D1-P64	UNIVERSAL	0025	103

ACE	MODEL	IMPLANT	PLATFORM	CODE	
	EXTERNAL HEX	3,3	NP 3,5	0023	99
		3,75/4	RP 4,1	0024	101
		4,75	WP 5	0058	163
	INFINITY TRI-CAM	3,5	3,5	0026	106
		4,3	4,3	0027	108
		5	5	0028	110
	INFINITY INTERNAL HEX	3,7/4,1	3,5	0040	131
		4,7/5,1	4,5	0041	136
	INFINITY OCTAGON	3,3	RP 4,8	0037	124
		4,1	RP 4,8	0037	124
		4,8	RP 4,8	0037	124
		4,8	WP 6,5	0096	201
	MULTI UNIT	Universal	UNIVERSAL	0025	103

ADIN	MODEL	IMPLANT	PLATFORM	CODE	
	SWELL	3,3	3,45	0040	131
		3,3	3,45	0042	131
		3,75/4,2	3,6	0040	131

## COMPATIBILITIES AVAILABLE

ADIN	MODEL	IMPLANT	PLATFORM	CODE	
	SWELL	3.75/4.2	3.6	0042	131
		5	4	0040	131
		5	4	0042	131
		6	4.6	0040	131
		6	4.6	0042	131
	TOUAREG-S / TOUAREG-OS	3.5	3.45	0040	131
		3.5	3.45	0042	131
		3.75/4.2	3.6	0040	131
		3.75/4.2	3.6	0042	131
		5	4	0040	131
		5	4	0042	131
		6	5	0040	131
		6	5	0042	131
	TOUAREG CLOSEFIT	2.75	UNP	0188	279
		3	NP	0145	239
		3.5	RP	0021	93
		4.3/5	WP	0022	96
	TRIPLE	3.5/3.75/4.2/5/6	STANDARD	0040	131
		3.5/3.75/4.2/5/6	STANDARD	0042	131
	MULTI UNIT TMA	Universal	UNIVERSAL	0025	103

ALFA-GATE	MODEL	IMPLANT	PLATFORM	CODE	
	BIOACTIVE/POROUS/ TRIO/MAX	3.3/3.75/4.2/ 4.7/5.2/6	SP	0040	131
	CONICAL	3.5	NP	0021	93
		4.3/5	RP	0022	96

ALPHABIO	MODEL	IMPLANT	PLATFORM	CODE	
	INTERNAL HEX CONNECTION (IH) SPI	3.3/3.75/4.2/5/6	UNIVERSAL	0040	131
	INTERNAL HEX CONNECTION (IH) ICE	3.7/3.75/4.2/ 4.65/5.3	UNIVERSAL	0040	131

## COMPATIBILITIES AVAILABLE



ALPHABIO	MODEL	IMPLANT	PLATFORM	CODE	
	INTERNAL HEX CONNECTION (IH) DFI	3.3/3.75/4.2/5	UNIVERSAL	0040	131
	INTERNAL HEX CONNECTION (IH) ATID	3.3/3.75/4.2/5/6	UNIVERSAL	0040	131
	INTERNAL HEX CONNECTION (IH) NEO	3.75/4.2/5	3.5	0040	131
	CONICAL HEX CONNECTION (CHC) NICE	3.2	NARROW	0136	236
	CONICAL HEX CONNECTION (CHC) NEO	3.2/3.5	NARROW	0136	236
	CONICAL STANDARD CONNECTION (CS)	3.75/4.2/5	STANDARD	0169	260
	MULTI UNIT ABUTMENT	-	UNIVERSAL	0195	285

ALPHA-DENT	MODEL	IMPLANT	PLATFORM	CODE	
	CLASSIC CONUS	3.3/3.75	3	0265	328
	ACTIVE CONUS	3.25/3.75	3	0265	328

ANCLADEN	MODEL	IMPLANT	PLATFORM	CODE	
	ANCLALOCK	3.75/4.25/5	3.5	0040	131

ANKLYOS	MODEL	IMPLANT	PLATFORM	CODE	
	ANKYLOS	3.5	3.5	0075	174
		4.5	4.5	0075	174
		5.5	5.5	0075	174
		7	7	0075	174
	BALANCE BASE NARROW	Universal	UNIVERSAL	0183	272

# COMPATIBILITIES AVAILABLE



ANTHOGYR	MODEL	IMPLANT	PLATFORM	CODE	
	AXIOM BL REG / PX	3,4	3,4	<b>0161</b>	250
		4	4	<b>0149</b>	240
		4,6	4,6	<b>0149</b>	240
		5,2	5,2	<b>0162</b>	252
	ANTHOFIT HE	3,5/3,75/4	R (4,1)	<b>0024</b>	101
		5	L (5)	<b>0058</b>	163
	OSSFIT	3,5/4,2	4,8	<b>0074</b>	172
		3,5/4,2	4,8	<b>0037</b>	124
		5	6,5	<b>0096</b>	201
	MULTI UNIT	4,8	UNIVERSAL	<b>0163</b>	254

ARDS	MODEL	IMPLANT	PLATFORM	CODE	
	SMART	3,75/4,2/4,5	3,75	<b>0040</b>	131
	CLASSIC	3,3/3,75/4,2/5/6	3,75	<b>0040</b>	131
	PREMIUM	3,3/3,75/4,2/5/6	3,75	<b>0040</b>	131
	CIT	3,3/3,75/4,2/5/6	3,75	<b>0040</b>	131

ASTRA	MODEL	IMPLANT	PLATFORM	CODE	
	YELLOW	3	YELLOW (X-ESTRECHA)	<b>0109</b>	208
	AQUA	3,5/4	AQUA(ESTRECHA)	<b>0004</b>	52
	LILAC	4,5/5	LILAC (ANCHA)	<b>0005</b>	55
	UNIABUTMENT CONO 20°	Regular/Wide	REGULAR/WIDE	<b>0066</b>	171
	UNIABUTMENT CONO 45°	Regular/Wide	REGULAR/WIDE	<b>0067</b>	
	EVOLUTION/ PRIMETAPER	3	3,0	<b>0090</b>	194
		3,6	3,6	<b>0006</b>	57
		4,2	4,2	<b>0007</b>	60
		4,8	4,8	<b>0091</b>	196
		5,4	5,4	<b>0092</b>	199

## COMPATIBILITIES AVAILABLE



ASTRA	MODEL	IMPLANT	PLATFORM	CODE	
ASTRA	DS OMNITAPER EV	3	XS	0090	194
		3.4	S	0006	57
		3.8	M	0007	60
		4.5	L	0091	196
		5.5	XL	0092	199
	MULTIBASE ABUTMENT (SMARTFIX CONCEPT)	-	UNIVERSAL	0258	318
AVINENT	MODEL	IMPLANT	PLATFORM	CODE	
AVINENT	HE/EC	3.3/3.5/4	3.5	0023	99
		3.3/3.8/4/4.2/ 4.8/4.5/5	4.1	0024	101
		4.8	5.1	0061	169
	HI/IC	3.1/3.5/4	3.5	0040_B	134
		3.3/3.8/4/4.2/ 4.8/4.5/5	4.1	0040_B	134
	TRANSEPITELIAL	-	REGULAR	0025	103
B&W	MODEL	IMPLANT	PLATFORM	CODE	
B&W	HEXÁGONO EXTERNO	3.75/4	4.1	0024	101
		5	5	0058	163
	CÓNICO HEXAGONO INTERNO CIH	3.3/4	4	0040	131
		3.3/4	4	0042	131
BEGO	MODEL	IMPLANT	PLATFORM	CODE	
BEGO	RS/R SX	3.0	3.0	0049	152
	S/RI/RS/R SX	3.25/3.75	3.67	0050	153
		4.1	4.1	0051	155
		4.5	4.5	0052	157
		5.5	5.5	0081	179
	MINI	2.7/2.9/3.1	MINI	0187	277
	MULTIPLUS	-	UNIVERSAL	0150	242

## COMPATIBILITIES AVAILABLE



BIOCONCEPT	MODEL	IMPLANT	PLATFORM	CODE	
	BC TISSUE LEVEL STANDARD	3.3/4.1/4.8	REGULAR	0037	124
	BC TISSUE LEVEL STANDARD PLUS	4.8	REGULAR	0037	124
	BC TISSUE LEVEL TAPERED EFFECT	4.8	REGULAR	0037	124
	BC BONE LEVEL	3.3	NARROW	0033	118
		4.1/4.8	REGULAR	0035	121
	BV TAPERED BONE LEVEL	3.5	NARROW	0029	112
		4/4.5/5	REGULAR	0030	115
BIOGENESIS	MODEL	IMPLANT	PLATFORM	CODE	
	3ICON	3.3	MINI (PINK)	0023	99
		3.75/4/4.3/4.5	REGULAR (BLUE)	0024	101
		5/5.5	WIDE (YELLOW)	0058	163
	ATICON	3.5/4/4.5/5	BLUE	0005	55
	ITICON	3.5/4.1/4.8	4.8	0037	124
BIOHORIZONS	MODEL	IMPLANT	PLATFORM	CODE	
	EXTERNAL	3.5	3.7 (YELLOW)	0023	99
	TAPERED INTERNAL	3/3.4	3 (GREY)	0102	205
		3.8	3.5 (YELLOW)	0040	131
		4.6	4.5 (GREEN)	0041	136
		5.8	5.7 (BLUE)	0080	177
	TAPERED PLUS	3.8	3 (GREY)	0102	205
		4.6	3.5 (YELLOW)	0040	131
		5.28	4.5 (GREEN)	0041	136
	MOUNT-FREE TAPERED INTERNAL	3/3.4	3 (GREY)	0102	205
		3.8	3.5 (YELLOW)	0040	131

## COMPATIBILITIES AVAILABLE



BIOHORIZONS	MODEL	IMPLANT	PLATFORM	CODE		
BIOHORIZONS	MOUNT-FREE TAPERED INTERNAL	4,6	4,5 (GREEN)	<b>0041</b>	136	
		5,8	5,7 (BLUE)	<b>0080</b>	177	
	TAPERED PRO	3,8	3 (GREY)	<b>0102</b>	205	
		4,2/4,6	3,5 (YELLOW)	<b>0040</b>	131	
		5,2	4,5 (GREEN)	<b>0041</b>	136	
	TAPERED SHORT	4,6	3,5 (YELLOW)	<b>0040</b>	131	
		5,8	4,5 (GREEN)	<b>0041</b>	136	
	TAPERED PTG	4,2	3,5 (YELLOW)	<b>0040</b>	131	
	TAPERED IM (INMEDIATE MOLAR)	7/8	5,7 (BLUE)	<b>0080</b>	177	
	TAPERED TISSUE LEVEL	3/3,8	3,5 (YELLOW)	<b>0040</b>	131	
		4,6	4,5 (GREEN)	<b>0041</b>	136	
		5,8	5,7 (BLUE)	<b>0080</b>	177	
	TAPERED PRO CONICAL	3,3/3,8	NARROW (GREY)	<b>0119</b>	214	
		4,2/4,6/5,2	REGULAR (YELLOW)	<b>0120</b>	217	
	MULTI UNIT	-	UNIVERSAL	<b>0025</b>	103	
	BIOMET 3i	OSSEOTITE EXTERNAL HEX	3,25	3,4	<b>0003</b>	50
			3,75/4	4,1	<b>0024</b>	101
			5	5	<b>0058</b>	163
			6	6	<b>0179</b>	
CERTAIN		3,25/4	3,4	<b>0001</b>	44	
		4/5	4,1	<b>0002</b>	47	
		5	5	<b>0057</b>	161	
LOW PROFILE		-	UNIVERSAL	<b>0025</b>	103	
BIOLOK		HEXÁGONO EXTERNO	3,45	3,45	<b>0003</b>	50

## COMPATIBILITIES AVAILABLE



BIONER	MODEL	IMPLANT	PLATFORM	CODE	
	IKELT / BIKELT	3.3/3.75/4	4.1	0024	101
	IKELT	5	5	0058	163
	HIKELT	3.8	3.95	0040	131
		4.7	4.9	0041	136
	TOPDM	3.5	3.5	0021	93
		4	4	0021	93
		5	5	0021	93
	SHORT DM	4/5/6	UNIVERSAL	0021	93
	HIBIKELT	4/5	UNIVERSAL	0021	93
	TRANSEPITELIAL A-5M	Transepitelial A-5M	REGULAR	0025	103

BIOTEC	MODEL	IMPLANT	PLATFORM	CODE	
	SPR/CIM	3.3	3.3	0040	131
		3.75	3.75	0040	131
	SPR/SPTT/CIM	4.2	4.2	0040	131
		5	5	0040	131

BIOTEM	MODEL	IMPLANT	PLATFORM	CODE	
	AR FIXTURE	3.7/4/4.5	REGULAR	0030	115

BRENT MEDICAL	MODEL	IMPLANT	PLATFORM	CODE	
	NARROW SKY	3.5	NP 3.5	0110	210
	BLUE SKY	3.5/4/4.5/5.5	4	0111	212
	BLUE SKY CLASSIC	3.5/4/4.5	4	0111	212
	COPA SKY	3.5/4/4.5/5/6	3.3	0251	314

## COMPATIBILITIES AVAILABLE

BTI	MODEL	IMPLANT	PLATFORM	CODE	
	EXTERNA TINY	2.5/3.9/3/3.3/ 3.5/3.75	TINY 3.5	0009	65
	EXTERNA UNIVERSAL	3.75/4	UNIVERSAL 4.1	0024	101
	EXTERNA UNIVERSAL PLUS	4.5/5	UNIVERSAL PLUS 4.1	0024	101
	EXTERNA	4.5/5/5.5	ANCHA 5.5	0060	167
	INTERNA	3.3/3.5/3.75	3.5	0257	317
	INTERNA UNIVERSAL	3.3/3.5/3.75/ 4/4.25	UNIVERSAL 4.1	0010	67
	INTERNA UNIVERSAL PLUS	4.5/5/5.5	UNIVERSAL PLUS 4.1	0010	67
	INTERNA ANCHA	5.5/6/6.25	ANCHA 5.5	0059	165
	MULTI-IM	converter 4.1	UNIVERSAL 4.1	0151	243
BTK	MODEL	IMPLANT	PLATFORM	CODE	
	KLASSIC / KONIC	3.25	3.4 EN	0003	50
	KLASSIC / KONIC/LINE PLUS	3.25PL/3.75/4	4.1 ER	0024	101
	IS +/LINE PLUS IS+	3.3/3.7/4.1/4.8/6	DR	0029	112
	BT SAFE BL	3.3/3.7/4.1/4.8	KR	0029	112
	KLASSIC / KONIC	3.25/4	3.5 IR	0040	131
		3.25/4	3.5 IR	0042	131
	LINE PLUS IC+	3.25/3.75/4.25/5	LR	0040	131
CAMLOG	MODEL	IMPLANT	PLATFORM	CODE	
	CAMLOG SCREW-LINE/ PROGRESSIVE-LINE	3.3	3.3	0087	190
		3.8	3.8	0011	69
		4.3	4.3	0012	72

## COMPATIBILITIES AVAILABLE

CAMLOG	MODEL	IMPLANT	PLATFORM	CODE	
	CAMLOG SCREW-LINE/ PROGRESSIVE-LINE	5	5	<b>0088</b>	192
		3.3	3.3	<b>0119</b>	214
		3.8	3.8	<b>0120</b>	217
		4.3	4.3	<b>0121</b>	220
CONEXÃO SISTEMA DE PRÓTESE	MODEL	IMPLANT	PLATFORM	CODE	
	NP 24° FLESH GOLD	3.5/3.75/4.3/5	UNIVERSAL	<b>0021</b>	127
	NP 24° FLASH	3.5/4.3/5	UNIVERSAL	<b>0021</b>	127
	NP 24° PTERYTRANS EX	3.5	UNIVERSAL	<b>0021</b>	127
	NP 24° SHORT® NP BLT	3.75/4.3	UNIVERSAL	<b>0021</b>	127
	NP 24° TORQ	3.5/3.75/4	UNIVERSAL	<b>0021</b>	127
	NP 24° EXPAND	3.75/4/5	UNIVERSAL	<b>0021</b>	127
CORTEX	MODEL	IMPLANT	PLATFORM	CODE	
	INTERNAL HEX DYNAMIX	3.3/3.8/4.2/5/6	3.75	<b>0040</b>	131
	INTERNAL HEX CLASSIX	3.3/3.8/4.2/5/6	3.75	<b>0040</b>	131
	INTERNAL HEX SATURN	3.8/4.2	3.5	<b>0040</b>	131
	CONICAL DYNAMIX	3	NP	<b>0109</b>	208
		3.3/3.8/4.2	RP	<b>0004</b>	52
		5/6	WP	<b>0005</b>	55
	CONICAL CLASSIX	3.3/3.8/4.2	RP	<b>0004</b>	52
		5/6	WP	<b>0005</b>	55
	CONICAL MAGIX	3.3/3.8/4.2	RP	<b>0004</b>	52
	MULTI UNIT	-	UNIVERSAL	<b>0025</b>	103
C-TECH	MODEL	IMPLANT	PLATFORM	CODE	
	EL ESTHETIC LINE	3.8/4.3/5.1	4	<b>0246</b>	309
	MULTI UNIT	-	UNIVERSAL	<b>0245</b>	308

## COMPATIBILITIES AVAILABLE



COWELMEDI	MODEL	IMPLANT	PLATFORM	CODE	
	INNO - SUBMERGED TYPE	3,5/4/4,5/5/6	UNIVERSAL	0030	115
	INNO - EXTERNAL TYPE	5,0/6,0	5.1	0061	169
	MULTI S&A ABUTMENT Ø 4,5 MM	Multi S Abutment	UNIVERSAL	0193	283
DENTAL TECH	MODEL	IMPLANT	PLATFORM	CODE	
	IMPLOGIC	4,5	4,5 (BLUE)	0041	136
DENTAURUM	MODEL	IMPLANT	PLATFORM	CODE	
	TIOLOGIC	3,3	SMALL	0130	231
		3,7/4,2	MEDIUM	0131	232
		4,8/5,5	LARGE	0132	233
DENTEGRIS	MODEL	IMPLANT	PLATFORM	CODE	
	SLS-STRAIGHT	4,5	4,5	0041_B	139
	SINUS-LIFT	4,5	4,5	0041_B	139
	S&T IMPLANTS	4,5	4,5	0041_B	139
DENTEM	MODEL	IMPLANT	PLATFORM	CODE	
	-	-	REGULAR	0030	115
DENTIS	MODEL	IMPLANT	PLATFORM	CODE	
	ONEQ-SL	3	NARROW	0014	76
		3,9/4,2/4,7/5,2	REGULAR	0030	115
		6/7/8	WIDE	0030	115
	S-CLEAN TAPERED / TAPERED II	3,7	MINI	0030	115
		4,1/4,3	REGULAR	0030	115
		4,8	WIDE	0030	115

## COMPATIBILITIES AVAILABLE



DENTIS	MODEL	IMPLANT	PLATFORM	CODE	
	S-CLEAN STRAIGHT	4,1/4,8	4,1/4,8	0030	115
	S-CLEAN SAVE	5,5/6	5,5/6	0030	115
	SQ-SL	3,5	NARROW	0014	76
		4/4,5/5	REGULAR	0030	115
		6/7/8	WIDE	0030	115
	E-CLEAN	3,5	MINI	0023	99
		4,1	REGULAR	0024	101
		5,1	WIDE	0061	169

DENTIUM	MODEL	IMPLANT	PLATFORM	CODE	
	NR LINE	3,1	3,2	0190	280
		3,1	3,6	0190	280
		3,6	3,6	0191	281
		4,3	4,3	0191	281
		5	5	0191	281
		6	6	0191	281
	MULTI UNIT NR LINE		5	0192	282
	SIMPLELINE II	3,8/4,3	4,8	0074	172
		3,8/4,3	4,8	0037	124
		4,3/4,8	6,5	0096	201
	SUPERLINE/SUPERLINE II/IMPLANTIUM	3,4	3,6	0030	115
		3,8	4	0030	115
		4,3	4,5	0030	115
		4,8	5	0030	115
		4,8	6	0030	115
	MULTI UNIT SUPERLINE AND IMPLANTIUM	-	4,5	0193	283

DIO IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	SM SYSTEM	3,8/4,1	NARROW	0076	
		4,5/5/5,3	REGULAR/WIDE	0013	75
	UF II NARROW	3/3,3	NARROW	0014	76

## COMPATIBILITIES AVAILABLE

DIO IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	UF II	3,8/4/4,5/5/5,5	REGULAR	0030	114
	EXTERNAL	3,3/3,8	NARROW 3,5	0023	99
		3,75/4/4,5	REGULAR 4,1	0024	101
		5/5,3/5,5/6	WIDE 5,1	0061	169
	INTERNAL OCTA	-	4,8	0074	172
	MULTI UNIT	-	UNIVERSAL	0247	310

DITRON	MODEL	IMPLANT	PLATFORM	CODE	
	ULTIMATE MATRIX	3,75/4,2	3,75	0040	131
		5	4	0040	131
		6	4,6	0040	131
	MPI MATRIX	3,5	3,5	0040	131
		3,75	3,75	0040	131
		4,2	4,2	0040	131
		5	5	0040	131
		6	6	0040	131

DMI DENTAL SUPPLY	MODEL	IMPLANT	PLATFORM	CODE	
	DCI/DSI	3,3/3,5/3,75/ 4,2/5/6	3,75	0040	131

DSP BIOMEDICAL	MODEL	IMPLANT	PLATFORM	CODE	
	HEXÁGONO EXTERNO	3,75/4/5/ 3,5/3,8/4,3	4,1	0024	101

EASY IMPLANT	MODEL	IMPLANT	PLATFORM	CODE	
	MASTER C	3,5	3,5 (OCEAN)	0004	52
		4	4 (OCEAN)	0004	52
		4,5	4,5 (LILAS)	0030	115
		5	5 (LILAS)	0030	115

## COMPATIBILITIES AVAILABLE



EASY IMPLANT	MODEL	IMPLANT	PLATFORM	CODE		
EASY IMPLANT	MASTER S	3,3	3,3 (OCEAN)	0004	52	
		3,75	3,75 (LILAS)	0030	115	
		4,25	4,25 (LILAS)	0030	115	
		4,75	4,75 (LILAS)	0030	115	
	MASTER L	3,3	3,3 (LILAS)	0030	115	
		3,75	3,75 (LILAS)	0030	115	
		4,25	4,25 (LILAS)	0030	115	
		4,75	4,75 (LILAS)	0030	115	
	MINI	3	3	0176	268	
	HEXCEL-S	3,3	3,3	0003	50	
		3,75	4,1	0024	101	
		4,25	4,1	0024	101	
		4,75	5	0058	163	
	MULTI UNIT CONICAL ABUTMENT	-	UNIVERSAL	0025	103	
	<hr/>					
	ECKERMANN	MODEL	IMPLANT	PLATFORM	CODE	
ECKERMANN	ALL-SPIRAL	4	REGULAR	0069		
	DUPLO	4	REGULAR	0070		
	HEXAGON	3/3,5/4/4,5/5	4,1	0024	101	
	WINNER	3/3,5/4	3,5	0040_B	134	
		3/3,5/4	3,5	0042	131	
		4/4,5/5	4,5	0041_B	139	
		4/4,5/5	4,5	0043		
	<hr/>					
ELITE MEDICA	MODEL	IMPLANT	PLATFORM	CODE		
ELITE MEDICA	CONEXIÓN EXTERNA	3,75	NARROW	0023	99	
		4	REGULAR	0024	101	
		5	WIDE	0061	169	

## COMPATIBILITIES AVAILABLE



EUROTEKNIKA	MODEL	IMPLANT	PLATFORM	CODE	
	NATURACTIS	3.5	3.4	0004	52
		4	3.8	0004	52
		4.5	4.3	0004	52
		5	4.8	0004	52
	UNEVA	3.6	4.1	0024	101
		4.1	4.1	0024	101
	UNEVA (PLATFORM SWITCHING)	4.8	4.1	0024	101
		6	4.1	0024	101
	NATEA	3,6/4,1/4,8	NARROW	0004	52
		3,6/4,1/4,8	REGULAR	0004	52
		6	WIDE	0004	52
	AESTHETICA	4.1	4.8	0074	172
		4.1	4.8	0037	124
		4.8	6.5	0096	201
	NATURALL	3.5	NARROW	0004	52
		4/4.5	REGULAR	0004	52
		5	WIDE	0004	52
	IBONE E/IBONE S	3,8/4,3/4,8	3.5	0004	52
		4,8/5,5/6,2	4.3	0004	52
	IBONE G	4,8/5,5	RP	0037	124
		5,5/6,2	WP	0096	201
MULTI UNIT TETRA	Universal	UNIVERSAL	0025	103	
F&B IMPLANT (FIT & BRILLIANT)	FA SUBMERGED FIXTURE	3.9	NARROW	0030	115
		4,1/4,4	REGULAR	0030	115
		4.8	WIDE	0030	115
		5,3/5,8/6,3/6,8	ULTRA-WIDE	0030	115
GALIMPLANT	CONEXIÓN EXTERNA	3.5/4	4	0024	101
		3.5	3.5	0004	52

## COMPATIBILITIES AVAILABLE



<b>GALIMPLANT</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	CONEXIÓN EXTERNA	4	4	<b>0004</b>	52
		5	5	<b>0004</b>	52
	PILAR MULTI-POSICION RECTO / PILAR MULTI-POSICION ANGULADO	Universal	UNIVERSAL	<b>0025</b>	103

---

<b>GC TECH</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	AADVA STANDARD / TAPERED IMPLANTS	3.3	NARROW	<b>0196</b>	287
		4	REGULAR	<b>0197</b>	288
		5	WIDE	<b>0198</b>	289

---

<b>GMI (ILERIMPLANT)</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	AVANTGARD	3.75/4.25	RP	<b>0243</b>	307
	PHOENIX	3.3/3.75/4	STANDARD 4.1	<b>0024</b>	101
		5	WIDE 5.1	<b>0061</b>	169
	FRONTIER	3.3/3.75/4.25	RP 3.3	<b>0040_B</b>	134
		4.75/5.75	WP 4.3	<b>0041_B</b>	139
	UNIVERSAL	Universal	PS-RP 4.8	<b>0025</b>	103

---

<b>GT MEDICAL</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	BEST FIT HEXÁGONO INTERNO	3.7/4.1/4.3/4.8	WIDE	<b>0005</b>	55
		3.7/4.3/4.8	REGULAR	<b>0074</b>	172
		3.7/4.3/4.8	REGULAR	<b>0037</b>	124
	BEST FIT HEXÁGONO EXTERNO	3.5	NARROW	<b>0023</b>	98
		4.1	REGULAR	<b>0024</b>	101
		5.1	WIDE	<b>0061</b>	169

---

<b>HAHN IMPLANT (GLIDEWELL)</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	HAHN TAPERED IMPLANT	3	3	<b>0159</b>	246
		3.5/4.3	3.5/4.3	<b>0021</b>	93
		5	5	<b>0022</b>	96
		7	7	<b>0124</b>	223
	MULTI-UNIT ABUTMENT SYSTEM	Universal	UNIVERSAL	<b>0025</b>	103

## COMPATIBILITIES AVAILABLE

HIOSSEN	MODEL	IMPLANT	PLATFORM	CODE	
	ETII SA / ETIII SA	3.5	MINI	0029	112
	ETII SA / ETIII SA / ETIV SA	4/4,5/5	REGULAR	0030	115
	ETIII BA	3.5	MINI	0029	112
		4/4,5/5	REGULAR	0030	115

HI-TEC	MODEL	IMPLANT	PLATFORM	CODE	
	TAPERED SELF THREAD	3.3/3.75	3.5	0040	131
		4.2/5	4.5	0041	136
	LOGIC PLUS	3.5	3.7	0040	131
		4.3	3.9	0040	131
		5/6	4.1	0040	131
	LOGIC / IMPLEX	3/3.5	3.5	0021	93
		3.5	3.9	0021	93
		4.3/5/6	3.9	0022	93

IBS	MODEL	IMPLANT	PLATFORM	CODE	
	MAGIC FC	4/4,5/5/5,5/ 6/6,5	3,8	0030	115
	N.R. FIX	3/3,5	3,8	0030	115

IDO IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	I Do Implant	3,8/4,4,5/5/ 5,5/6/7	UNIVERSAL	0030	115

IHDE DENTAL (IMBIODENT)	MODEL	IMPLANT	PLATFORM	CODE	
	BONE LEVEL PLUS	3.3	3.3	0033	118
		4.1	4.1	0035	121
		4.8	4.8	0035	121

## COMPATIBILITIES AVAILABLE

IMPLANT DIRECT	MODEL	IMPLANT	PLATFORM	CODE	
IMPLANT DIRECT	REPLUS / REPLANT / REACTIVE	3,5/3,7/4,2	3,5	<b>0026</b>	106
		4,3/4,7	4,3	<b>0027</b>	108
		5/5,7	5	<b>0028</b>	110
	LEGACY	3,7/4,2	3,5	<b>0040</b>	131
		4,7/5,2	4,5	<b>0041</b>	136
	SWISHPLANT / SWISHPLUS	4,1/4,8	4,8	<b>0074</b>	172
		4,1/4,8	4,8	<b>0037</b>	124
		4,8/5,7	6,5	<b>0096</b>	201
	SWISHACTIVE	3,3	3	<b>0021</b>	93
		4,1/4,8	3,4	<b>0022</b>	96
	INTERACTIVE	3,2/3,7	3	<b>0021</b>	93
		4,3/5	3,4	<b>0022</b>	96
	SIMPLY ICONIC	3,2/3,7/4,2	PURPLE 3,0	<b>0021</b>	93
		4,7/5,2/5,7	GOLD 3,4	<b>0022</b>	96
	MULTI UNIT ABUTMENT	-	5	<b>0158</b>	245
IMPLANT GENESIS	MODEL	IMPLANT	PLATFORM	CODE	
IMPLANT GENESIS	AKTIV SYSTEM	3,5/3,75/4,2/5	STANDARD	<b>0040</b>	131
IMPLANTSWISS	MODEL	IMPLANT	PLATFORM	CODE	
IMPLANTSWISS	BONE LEVEL	3,3	3,3	<b>0004</b>	52
		3,7	3,7	<b>0030</b>	115
		4,3	4,3	<b>0030</b>	115
		4,8	4,8	<b>0030</b>	115
		5,5	5,5	<b>0030</b>	115
	MULTI UNIT ABUTMENT	Universal	4,8	<b>0025</b>	103
INTRA-LOCK	MODEL	IMPLANT	PLATFORM	CODE	
INTRA-LOCK	UNIHEX	4	REGULAR	<b>0024</b>	101
		4,75	WIDE	<b>0024</b>	101
	INTRAHEX	3,75/4	3,5	<b>0040</b>	131
		4,75	4,5	<b>0041</b>	136

## COMPATIBILITIES AVAILABLE



JDENTALCARE	MODEL	IMPLANT	PLATFORM	CODE	
JDEVOLUTION/ JDEVOLUTION PLUS		3.7	3.7	0040	131
		4.3/5	4	0040	131
		6	5	0040	131
JD PTERYGO		4	4	0040	131
JD ICON/JD ICON F		3.9	3.9	0022	96
		4.3	4	0022	96
		5	4.7	0022	96
JD ICON PLUS		3.7	3.7	0015	79
		4.3	4	0015	79
		5	4.8	0015	79
JD ICON PLUS T		3.5	3.5	0015	79
		4	3.5	0015	79
		4.5	3.5	0015	79
CONICAL ABUTMENT		-	UNIVERSAL	0025	103

KEYSTONE	MODEL	IMPLANT	PLATFORM	CODE	
RESTORE		3.75/4	RD 4.1	0024	101
		5/6	WD 5	0061	169
INTERNAL TILOBE PRIMA CONNEX		3.3/3.5	3.5	0044	141
		4/4.1	4.1	0045	143
		5	5	0046	145
INTERNAL TILOBE PRIMA PLUS		3.5	3.5	0044	141
		4.1	4.1	0045	143
		5/6	5	0046	145

KLOCKNER	MODEL	IMPLANT	PLATFORM	CODE	
ESSENTIAL CONE		3.5/4/4.5	4.5	0054	159
		4.8	6	0071	
ESSENTIAL CONE PILAR 25°		3.5/4/4.5	4.5	0054	159
ESSENTIAL CONE OCTACONE 12°		3.5/4/4.5	4.5	0054	159

## COMPATIBILITIES AVAILABLE



KLOCKNER	MODEL	IMPLANT	PLATFORM	CODE	
	KL	3.3	NARROW	0023	99
		3,7/4,2	REGULAR	0024	101
		4.7	WIDE	0061	169
	VEGA	3.5	NV	0082	181
		4/4.5	RV	0083	183
	VEGA+	3,6	NV	0082	181
		4,1/4,6	RV	0083	183
	MULTI UNIT PERMANENT	4.2	UNIVERSAL	0173	267

KUWOTECH	MODEL	IMPLANT	PLATFORM	CODE	
	KISPLANT	3.5	SMALL	0030	115
		4/4.5/5/5.5/6	REGULAR&WIDE	0030	115

LASAK	MODEL	IMPLANT	PLATFORM	CODE	
	BIONIQ	2,9	QN (AMARILLO)	0166	256
		3.5	QR (AZUL)	0167	258
		4	QR (AZUL)	0167	258
		5	QR (AZUL)	0167	258

LEADER	MODEL	IMPLANT	PLATFORM	CODE	
	TIXOS INTERNAL HEX	3.3	3.5	0040	131
		3.75	4	0040	131
		3.3/3.75	4.1	0024	101
		5	5	0058	163

MEDENTIKA	MODEL	IMPLANT	PLATFORM	CODE	
	MULTI UNIT	-	UNIVERSAL	0025	103

MEDENTIS	MODEL	IMPLANT	PLATFORM	CODE	
	PREMIUM / ACTIVE MASTER	3.3	3.3 (PINK)	0249	312
		3.75	3.75 (RED)	0125	225

## COMPATIBILITIES AVAILABLE



MEDENTIS	MODEL	IMPLANT	PLATFORM	CODE	
	PREMIUM / ACTIVE MASTER	4,1	4,1 (GREEN)	<b>0125</b>	225
		4,8	4,8 (BLUE)	<b>0125</b>	225
	MULTI UNIT	-	UNIVERSAL	<b>0025</b>	103

MEGAGEN	MODEL	IMPLANT	PLATFORM	CODE	
	ANYRIDGE	3,5	SMALL	<b>0015</b>	79
		4/4,5	REGULAR	<b>0015</b>	79
		5/5,5	WIDE	<b>0015</b>	79
	ANYONE INTERNAL	3,5/4/4,5/5/6/7	GENERAL	<b>0030</b>	115
	ANYONE EXTERNAL	3,5	SMALL 3,5	<b>0023</b>	99
		4	REGULAR 4,1	<b>0024</b>	101
		4,5	REGULAR 4,5	<b>0024</b>	101
		5	WIDE 5	<b>0058</b>	163
		6	SUPERWIDE 5,5	<b>0058</b>	163
	CONE ABUTMENT	Universal	3,8	<b>0128</b>	228
		Universal	4,8	<b>0074</b>	172
	MINI NARROW RIDGE	3/3,4	MINI	<b>0014</b>	76
	EXFEEL	3,5	SMALL	<b>0037</b>	124
		4,1	REGULAR	<b>0037</b>	124
		4,8/5	WIDE	<b>0037</b>	124
	BLUE DIAMOND/BD CUFF/ANYRIDGE OCTA	3,3/3,7	NC	<b>0222</b>	297
		4,1/4,4/4,8/5,3/ 5,8/6,3	RC	<b>0223</b>	299
	MULTI UNIT N TYPE	Multi Unit N Type	UNIVERSAL	<b>0025</b>	103
	MULTI UNIT S TYPE	Multi Unit S Type	UNIVERSAL	<b>0264</b>	327

MICRODENT	MODEL	IMPLANT	PLATFORM	CODE	
	UNIVERSAL	2,8/3,25	3,5	<b>0003</b>	50
		3,3/3,5/3,75/4	4,1	<b>0024</b>	101
		4,2/5	5,1	<b>0058</b>	163
	SYSTEM	2,8/3,25	3,5	<b>0003</b>	50
	EKTOS	3,7/4,2	3,5	<b>0040_B</b>	134

## COMPATIBILITIES AVAILABLE

MIS	MODEL	IMPLANT	PLATFORM	CODE		
	LANCE	3,75/4,2	STANDARD	<b>0024</b>	101	
		5	WIDE	<b>0058</b>	163	
	MULTI-UNIT	-	GENERAL	<b>0020</b>	91	
		SEVEN	3,3	NARROW	<b>0019</b>	89
	3,75/4,2		STANDARD	<b>0040</b>	131	
	5/6		WIDE	<b>0041</b>	136	
	M4	3,3	NARROW	<b>0019</b>	89	
		3,75/4,2	STANDARD	<b>0040</b>	131	
		5/6	WIDE	<b>0041</b>	136	
	C1	3,3	NARROW	<b>0016</b>	82	
		3,75/4,2	STANDARD	<b>0017</b>	84	
		5	WIDE	<b>0018</b>	87	
	V3	3,9/4,3/5	STANDARD	<b>0017</b>	84	
	MONOIMPLANT	MODEL	IMPLANT	PLATFORM	CODE	
		MONOIMPLANT MULTI UNIT	3/3,7/4,1	4,8	<b>0025</b>	103
MOZO-GRAU (TICARE)	MODEL	IMPLANT	PLATFORM	CODE		
	MG OSSEOUS	3,3	3,4 MINI	<b>0003</b>	50	
		3,4/3,75/4,25	4,1 STANDARD	<b>0024</b>	101	
		5	5 MAXI	<b>0061</b>	169	
	MG INHEX	-	CON 45°	<b>0067</b>		
		3,3	2,3 MINI	<b>0109</b>	208	
		3,75/4,25	2,8 STANDARD	<b>0004</b>	52	
		5	3,8 MAXI	<b>0005</b>	55	
	MPI	MODEL	IMPLANT	PLATFORM	CODE	
		CONEXIÓN EXTERNA HE PRIVILEGE	3,3	3,5	<b>0009</b>	65
3,3/4			4,1	<b>0024</b>	101	
5			5	<b>0058</b>	163	
PRIVILEGE CM		3,5/4	REGULAR	<b>0004</b>	52	
		5	WIDE	<b>0005</b>	55	

## COMPATIBILITIES AVAILABLE

MPI	MODEL	IMPLANT	PLATFORM	CODE	
	EXCELLENCE CM	3,5/4	REGULAR	0004	52
		5	WIDE	0005	55
NEOBIOTECH	MODEL	IMPLANT	PLATFORM	CODE	
	EB EXTERNAL SYSTEM	3,5	NARROW	0023	99
	IS IMPLANT SYSTEM	3,2	S-NARROW	0029	112
		3,5	NARROW	0030	115
		4	REGULAR	0030	115
		4,5	REGULAR	0030	115
		5	WIDE	0030	115
		-	4,8	0025	103
NEODENT	MODEL	IMPLANT	PLATFORM	CODE	
	HELIX GM/DRIVE GM/ TITAMAX GM	3,5/3,75/4/ 4,3/5/6	REGULAR	0186	274
	SMART HE	3,75/4	4,1	0024	101
	HELIX HE	3,75/4/4,3	4,1	0024	101
	MINI PILAR CM / MINI PILAR ANGULADO CM	Mini Pilar CM / Mini Pilar Angulado CM	UNIVERSAL	0025	103
NEOSS	MODEL	IMPLANT	PLATFORM	CODE	
	PROACTIVE STRAIGHT/ TAPERED/EDGE	3,25 Royal Blue	3,25	0144	
		3,5 Green	STANDARD	0047	147
		4 Yellow	STANDARD	0047	147
		4,5 Blue	STANDARD	0048	149
		5 Peach	STANDARD	0048	149
		5,5 Lilac	STANDARD	0048	149
	PROACTIVE WIDE	6	STANDARD	0048	149
	PROACTIVE SINUS	6,5	STANDARD	0048	149
	SHORT IMPLANT	3,5/4/4,5	STANDARD	0047	147
		5/5,5/6/6,5	STANDARD	0048	149

## COMPATIBILITIES AVAILABLE



NOBEL BIOCARE	MODEL	IMPLANT	PLATFORM	CODE	
NOBEL BIOCARE	BRANEMARK	3.3	NARROW	<b>0023</b>	99
		3.75/4	REGULAR	<b>0024</b>	101
		5/6	WIDE	<b>0061</b>	169
	REPLACE	3.5	NARROW	<b>0026</b>	106
		4.3	REGULAR	<b>0027</b>	108
		5	WIDE	<b>0028</b>	110
		6	PLATFORM 6	<b>0129</b>	229
	ACTIVE/REPLACE CONICAL CONNECTION	3	MINI 3.0	<b>0159</b>	246
		3.5	NARROW	<b>0021</b>	93
		4.3/5	REGULAR	<b>0022</b>	96
		5.5	WIDE	<b>0124</b>	223
	NOBELSPEEDY	3.3	NARROW	<b>0023</b>	99
		4/5	REGULAR	<b>0024</b>	101
		5/6	WIDE	<b>0061</b>	169
	NOBEL BIOCARE	MODEL	IMPLANT	PLATFORM	CODE
NOBEL BIOCARE	NOBELPARALLEL	3.75	NARROW	<b>0021</b>	93
		4.3/5	REGULAR	<b>0022</b>	96
		5.5	WIDE	<b>0124</b>	223
NORIS MEDICAL	MODEL	IMPLANT	PLATFORM	CODE	
NORIS MEDICAL	TUFF	3.3/3.75/4.2/5/6	3.75	<b>0040</b>	131
	TUFF TT	3.3/3.75/4.2/5/6	3.75	<b>0040</b>	131
	ONIX	3.3/3.75/4.2/5/6	3.75	<b>0040</b>	131
	CORTICAL	4.0/5/6	3.75	<b>0040</b>	131
	PTERYCORE	4.2	3.75	<b>0040</b>	131
	PTERYFIT	4.2	3.75	<b>0040</b>	131
NORMON	MODEL	IMPLANT	PLATFORM	CODE	
NORMON	NORMOIMPLANT HE	3.25/3.75/4.25/ 4.75	4.1	<b>0024</b>	101
	NORMOIMPLANT HI	3.75/4.25/4.75	3.5	<b>0040_B</b>	134

## COMPATIBILITIES AVAILABLE

NOVA IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	PSI/PCI	3.3/3.75/4.2/5/6	3.75	<b>0040_B</b>	134

OSSTEM IMPLANT	MODEL	IMPLANT	PLATFORM	CODE	
	TS	3	MINI 3.0	<b>0029</b>	112
		3.5	MINI 3.5	<b>0029</b>	112
		4/4.5/5/6/7	REGULAR	<b>0030</b>	115
	US	3.3/3.5	MINI 3.5	<b>0023</b>	99
		3.75/4/4.5	REGULAR 4.1	<b>0024</b>	101
		5/5.5	WIDE 5.1	<b>0061</b>	169
		5/5.5	WIDE PS 5	<b>0058</b>	162
	MULTI UNIT ABUTMENT/ESTHETIC LOW ABUTMENT	Universal	MINI/REGULAR	<b>0025</b>	103

OSTEOPLUS	MODEL	IMPLANT	PLATFORM	CODE	
	SHE	3.45	3.45	<b>0009</b>	65
		3.75 / 4	4	<b>0024</b>	101
	SHI	3.3 / 3.75 / 4.2	3.5	<b>0040</b>	131

OXY	MODEL	IMPLANT	PLATFORM	CODE	
	K1 LINE	3.5/4/4.5/5	REGULAR	<b>0015</b>	79
		5.5/6/6.5	WIDE	<b>0015</b>	79
	PSK LINE	3.5/4/4.5/5	REGULAR	<b>0015</b>	79
	MD LINE KONE	3.75/4.25/5	REGULAR	<b>0015</b>	79
	MD LINE EXT	3.75/4.25	STANDARD	<b>0024</b>	101
	FIXO	Universal	4.8	<b>0242</b>	305

PALTOP	MODEL	IMPLANT	PLATFORM	CODE	
	ADVANCED CLASSIC	3.25	NARROW (BLUE)	<b>0229</b>	302
		3.75/4.2/5	STANDARD	<b>0040_B</b>	134

## COMPATIBILITIES AVAILABLE



PALTOP	MODEL	IMPLANT	PLATFORM	CODE	
ADVANCED CLASSIC		3,75/4,2/5	STANDARD	<b>0042</b>	131
		6	WIDE (PURPLE)	<b>0041</b>	136
ADVANCED +		3,25	NARROW (BLUE)	<b>0229</b>	302
		3,75/4,2/5	STANDARD	<b>0040_B</b>	134
		3,75/4,2/5	STANDARD	<b>0042</b>	131
		6	WIDE (PURPLE)	<b>0041</b>	136
DYNAMIC		3,25	NARROW (BLUE)	<b>0229</b>	302
		3,75/4,2/5	STANDARD	<b>0040_B</b>	134
		3,75/4,2/5	STANDARD	<b>0042</b>	131
		6	WIDE (PURPLE)	<b>0041</b>	136
PAI		3,25	NARROW (BLUE)	<b>0229</b>	302
		3,75/4,2/5	STANDARD	<b>0040_B</b>	134
		3,75/4,2/5	STANDARD	<b>0042</b>	131
		6	WIDE (PURPLE)	<b>0041</b>	136
DIVA/ACTIVE		3,75/4,2/5	STANDARD	<b>0040_B</b>	134
		3,75/4,2/5	STANDARD	<b>0042</b>	131
CONICAL ACTIVE		3,25/3,75/4,2/5	STANDARD	<b>0029/0182</b>	112
UNIVERSAL MULTI-UNIT		Multi-Unit	UNIVERSAL	<b>0181</b>	270

P-I BRANEMARK	MODEL	IMPLANT	PLATFORM	CODE	
MT		3,3	3,5 (RED)	<b>0178</b>	269
		3,75	4,1 (GREEN)	<b>0178</b>	269
		4,8	5,1 (YELLOW)	<b>0178</b>	269

PHIBO	MODEL	IMPLANT	PLATFORM	CODE	
TSH/BNT SERIE 3		3,6	4	<b>0024</b>	101
TSH/BNT SERIE 4		4,2	4	<b>0024</b>	101

POINT IMPLANT	MODEL	IMPLANT	PLATFORM	CODE	
SM II SYSTEM UV IMPLANT		4/4,5/5	REGULAR	<b>0030</b>	115

## COMPATIBILITIES AVAILABLE



PROCLINIC	MODEL	IMPLANT	PLATFORM	CODE	
	CILINDRICO EXTERNO	3.3	3.3 MINI	0009	65
	CILINDRICO EXTERNO/ CÓNICO EXTERNO	3.75/4.25/3.5/4	4.1 ESTANDAR	0024	101
		5	5 MAXI	0058	163
		3.3/3.75/4.25/5/ 3.5/4/5	3.5	0040	131
	SP OCTA	3.3/4.1/4.8	4.8	0074	172
		3.3/4.1/4.8	4.8	0037	124
		4.8	6.5	0096	201
	AQUA CM	3.5/4/5	2.82	0004	52

PROTEG IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	PR01	3.3/3.75/4.2/5/6	NARROW	0265	328

RADHEX	MODEL	IMPLANT	PLATFORM	CODE	
	PHE	3.5	3.5	0023	99
		4/4.5/5	4.1	0024	101
	PHI	3.75	3.5	0040_B	134
		4.5/5	4.5	0041_B	139

REFLECT	MODEL	IMPLANT	PLATFORM	CODE	
	RAPID	3.0	3.0	0159	246
		3.5	NP	0021	93
		4.3/5/5.5	RP	0022	96
	RECOVER	3.5	NP	0021	93
		4.3/5	RP	0022	96
	ASPIRE	3.5/4	AQUA (ESTRECHA)	0004	51
		5	LILAC (ANCHA)	0005	54
	TAPERED SCREW	3.5	3.5	0040	131
		4.1/4.7	4.5	0041	136

## COMPATIBILITIES AVAILABLE

RITTER	MODEL	IMPLANT	PLATFORM	CODE	
	SB/LA/QSI	3,75/4,2/5/6	STANDARD	<b>0040_B</b>	134
ROOTT	MODEL	IMPLANT	PLATFORM	CODE	
	R	3,5/3,8/4,2/ 4,8/5,5	UNIVERSAL	<b>0236</b>	303
SEWON MEDIX	MODEL	IMPLANT	PLATFORM	CODE	
	IH <sub>2</sub> SLA SYSTEM	3,5	MINI	<b>0029</b>	112
		3,5/4/4,5/5	REGULAR	<b>0030</b>	115
	IH <sub>2</sub> RBM SYSTEM	3,5	MINI	<b>0029</b>	112
		3,5/4/4,5/5	REGULAR	<b>0030</b>	115
	IH SYSTEM	3,5/4/4,5/5	UNIVERSAL	<b>0025</b>	103
SIC INVENT	MODEL	IMPLANT	PLATFORM	CODE	
	HEXAGONAL SYSTEM SICACE	3,4/4	3,3	<b>0170</b>	263
		4,5/5	4,2	<b>0171</b>	265
	HEXAGONAL SYSTEM SICMAX	3,4/4,2	3,3	<b>0170</b>	263
		4,7/5,2	4,2	<b>0171</b>	265
	HEXAGONAL SYSTEM SICTAPERED	3,4/4,2	3,3	<b>0170</b>	263
		4,7/5,2	4,2	<b>0171</b>	265
SIGNO VINCES	MODEL	IMPLANT	PLATFORM	CODE	
	DUO	4,6	4,1	<b>0024</b>	101
	INTTEGRA	3,75/4	4,1	<b>0024</b>	101
	COMPACT	4,5	CM3,8	<b>0004</b>	51
	DUOCON	3,8	CM3,8	<b>0004</b>	51
		4,6/5,5	CM4,6	<b>0005</b>	54
	INFRA	3,3/3,8/4,6	CM	<b>0004</b>	51

## COMPATIBILITIES AVAILABLE

SIN IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	HE	3.75	4.1	0024	101
	HI SW	3.8	3.8	0039	129
	TRYON	3.25/3.75/4	4.1	0024	101
	TRYON CO	4	4.1	0024	101
	REVOLUTION	3.25/3.75/4	4.1	0024	101
	STYLUS	4	4.1	0024	101
	EPIKUT/EPIKUT PLUS	4.5	4.5	0024	101
		5	5	0058	163
	MINI PILAR	Universal	UNIVERSAL	0025	103
SOUTHERN IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	TRI-NEX	3.5	3.5	0026	106
		4.3	4.3	0027	108
		5	5	0028	110
		6	6	0129	229
	IT CONNECTION	3.3/4/4.1/4.9/5	4.8	0037	124
		4.9/5/6	6.5	0096	201
	EXTERNAL HEX	3.25	3.4	0003	49
		3.75/4	4.1	0024	101
		4.7/5	5	0058	163
		5.7/6	6	0058	163
	DEEP CONICAL	3	2.45	0109	208
		3.5/4	2.95/3.1	0004	52
		5	4.1	0005	55
	INTERNAL HEX	3.75/4.2/5	UNIVERSAL	0040	131
	PROVATA	4/5/6	STANDARD	0040	131
	COMPACT CONICAL	4.8	4.8	0025	103

## COMPATIBILITIES AVAILABLE



STERI-OSS	MODEL	IMPLANT	PLATFORM	CODE	
	HEX-LOC	3,25	3,3	<b>0023</b>	99
STERNGOLD	MODEL	IMPLANT	PLATFORM	CODE	
	STERN EX	3,75/4/5	4,1	<b>0024</b>	101
STRAUMANN	MODEL	IMPLANT	PLATFORM	CODE	
TISSUE LEVEL		3,3	3,5	<b>0160</b>	248
		3,3/4,1/4,8	REGULAR 4,8	<b>0037</b>	124
		4,8	WIDE 6,5	<b>0096</b>	201
SYNOCTA		-	REGULAR 4,8	<b>0074</b>	172
		-	WIDE 6,5	<b>0137</b>	238
BONE LEVEL TAPERED SC		2,9	SC- 2,9	<b>0135</b>	234
BONE LEVEL		3,3	NC- 3,3	<b>0033</b>	118
		4,1	RC-4,1	<b>0035</b>	121
		4,8	RC-4,8	<b>0035</b>	121
SCREW-RETAINED		NC/RC Ø4,6	UNIVERSAL	<b>0101</b>	203
BLX		3,5/3,75/4/4,5	RB (REGULAR BASE)	<b>0207</b>	292
		5/5,5/6,5	WB (WIDE BASE)	<b>0208</b>	295
BLC		3,3/3,75	RB	<b>0207</b>	292
		4,5/5,5/6,5	WB	<b>0208</b>	295
TLX / TLX S		3,75/4,5	NT	<b>0260</b>	321
		3,75/4,5	RT	<b>0261</b>	323
		5,5/6,5	WT	<b>0262</b>	325
TLC		3,3	NT	<b>0260</b>	321
		3,3/3,75/4,5	RT	<b>0261</b>	323
		4,5/5,5/6,5	WT	<b>0262</b>	325
SURCAM DENTAL	MODEL	IMPLANT	PLATFORM	CODE	
	MULTI-UNIT	-	UNIVERSAL	<b>0181</b>	270

## COMPATIBILITIES AVAILABLE



SYBRON IMPLANT SOLUTIONS	MODEL	IMPLANT	PLATFORM	CODE	
	ENDOPORE (INNOVA)	4.1	4.1	<b>0024</b>	101
SYSTHEX	MODEL	IMPLANT	PLATFORM	CODE	
	CLASSIC-CI / ESTETIC-CI	3.5/3.75/4	4.1	<b>0024</b>	101
TBR	MODEL	IMPLANT	PLATFORM	CODE	
	HEX-CONIC	3.5	NARROW	<b>0023</b>	99
		5	WIDE	<b>0058</b>	163
	CONNECT / INFINITY	3.5	3.5	<b>0266</b>	329
		4	4	<b>0267</b>	330
		5	5	<b>0268</b>	331
	BABY 8	4	4	<b>0267</b>	330
		5	5	<b>0268</b>	331
TITANIUM-FIX	MODEL	IMPLANT	PLATFORM	CODE	
	B-FIX	3.5/4	REGULAR	<b>0004</b>	51
		4.5/5	LARGA	<b>0005</b>	54
TREE-OSS	MODEL	IMPLANT	PLATFORM	CODE	
	SIMPLE	3.3/3.75/5	3.75 AMARILLO	<b>0040</b>	131
	RAPID/ANATOMIC	3.3	3.5 ROSA	<b>0023</b>	99
		3.75/4	4.1 AMARILLO	<b>0024</b>	101
		5	5.1 AZUL	<b>0061</b>	169
	ANATOMIC/HS	3.5	3.5 ROSA	<b>0026</b>	106
		4.3	4.3 AMARILLO	<b>0027</b>	108
		5	5 AZUL	<b>0028</b>	110
	MULTI UNIT	-	UNIVERSAL	<b>0025</b>	103

## COMPATIBILITIES AVAILABLE



TRI DENTAL IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	TRI-VENT	3.75/4.1/4.7	3.5	0040	131
		3.75/4.1/4.7	3.5	0042	131

---

TRINON	MODEL	IMPLANT	PLATFORM	CODE	
	Q2	3.5/3.75/4.5	4	0024	101
	QK	4	4.8	0074	172
		4	4.8	0037	124

---

UFIT	MODEL	IMPLANT	PLATFORM	CODE	
	GT2	3.5	MINI	0004	51
		4/4.5	REGULAR	0005	54
		5	WIDE	0005	54
		5.5/6/6.5/7	ULTRA-WIDE	0005	54
	NT2	3.5	MINI	0004	51
		4/4.5	REGULAR	0005	54
		5	WIDE	0005	54
		5.5/6/6.5/7	ULTRA-WIDE	0005	54

---

VULKAN IMPLANTS	MODEL	IMPLANT	PLATFORM	CODE	
	IN-HEX	3.3/3.75/4.2/5	3.75	0040	131

---

WARANTEC (ONEPLANT)	MODEL	IMPLANT	PLATFORM	CODE	
	IU IMPLANT SYSTEM	3.3/3.6	MINI	0004	51
		3.6	MINI	0004	51

---

WIN	MODEL	IMPLANT	PLATFORM	CODE	
	WIN	3.30/3.75/4.25/5	3.75	0040_B	134
		Universal	UNIVERSAL	0025	103

## COMPATIBILITIES AVAILABLE

<b>XIVE</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	XIVE	3	3	<b>0084</b>	185
		3.4	3.4	<b>0038</b>	127
		3.8	3.8	<b>0039</b>	129
		4.5	4.5	<b>0085</b>	186
		5.5	5.5	<b>0086</b>	188

---

<b>YES IMPLANT</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	S-SYSTEM	3.3/3.5	NARROW	<b>0030</b>	115
		4/4.5	REGULAR	<b>0030</b>	115
		5/5.5	WIDE	<b>0030</b>	115

---

<b>YOUSE IMPLANTS</b> <small>(Sweden &amp; Martina Group)</small>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	YOUSE-V/YOUSE-VL	3.3/3.7	NARROW	<b>0021</b>	93
		4.2/5	REGULAR	<b>0022</b>	96

---


<b>ZIACOM</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	OEX	3.75/4.25	RP 4.1	<b>0024</b>	101
	ZINIC	3.7/4/4.3	RP 3.5	<b>0040_B</b>	134
	ZINIC SHORTY	4.75	RP 3.5	<b>0040_B</b>	134
	GALAXY	3.4/3.7/4	RP 2.85	<b>0004</b>	51

---

<b>ZIMMER</b>	<b>MODEL</b>	<b>IMPLANT</b>	<b>PLATFORM</b>	<b>CODE</b>	
	SCREW-VENT	3.7/4.1	3.5	<b>0040</b>	131
		3.7/4.1	3.5	<b>0042</b>	131
		4.7	4.5	<b>0041</b>	136
		4.7	4.5	<b>0043</b>	
		6	5.7	<b>0080</b>	177
	TSX IMPLANT	3.1	2.9	<b>0178</b>	269
		3.7/4.1/4.7	3.5	<b>0040</b>	131
		3.7/4.1/4.7	3.5	<b>0042</b>	131

## COMPATIBILITIES AVAILABLE

ZIMMER	MODEL	IMPLANT	PLATFORM	CODE	
	TSX IMPLANT	5,4/6	4,5	<b>0041</b>	136
	SWISS-PLUS	3,7/4,1/4,8	4,8	<b>0074</b>	172
		3,7/4,1/4,8	4,8	<b>0037</b>	124
	EZTETIC	3,1	2,9	<b>0178</b>	269
	TAPERED ABUTMENT	Universal	UNIVERSAL	<b>0205</b>	290



This printed version is probably outdated and may not include all products or compatibilities.

**Scan and download the latest version of this catalogue**

[www.dynamicabutment.com](http://www.dynamicabutment.com)




# MULTI-UNIT DAS SYSTEM

# DYNAMIC DAS SYSTEM

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_1$  = Standard maximum angulation  $\alpha_2$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

# COMPATIBLE WITH 0001

LIST OF COMPATIBILITIES **AVAILABLE**  
BIOMET 3i

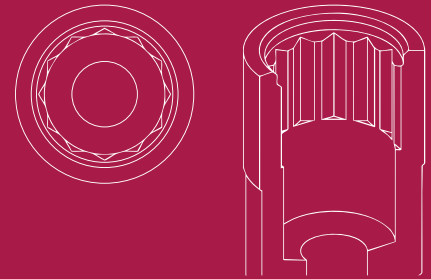

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	43°	29°	31.322.001.01-2	31.312.001.01-2
1,2	25°	22°	31.322.001.02-2	31.312.001.02-2
2	25°	-	31.322.001.03-2	31.312.001.03-2
3	20°	-	31.322.001.04-2	31.312.001.04-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,3	25°	20°	10°	31.322.001.21-2	31.312.001.21-2
2	25°	20°	10°	-	31.312.001.23-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.312.001.01-2	43.621.410.01-2
12	52.412.103.01-2	50.312.001.04-2 (IG=3mm)	43.624.410.01-2



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.001.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**


**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.754.01-2	22.612.001.01-2	34.612.001.01-2
4	25°	33.490.754.01-2		
6		33.690.754.01-2		



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.001.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		

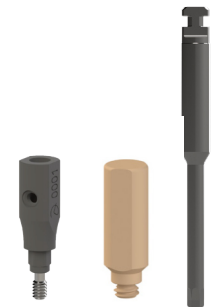

**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.084.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.003.01-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation


## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.001.01-2
2	42.302.001.02-2
3	42.302.001.03-2
4	42.302.001.04-2

[VIEW COMPONENTS](#)



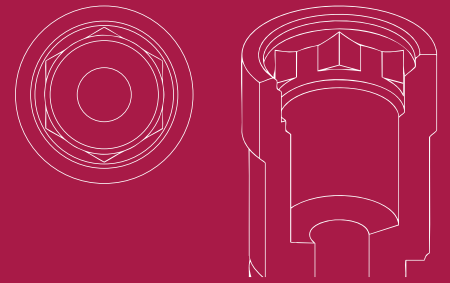

# COMPATIBLE WITH 0002

## LIST OF COMPATIBILITIES AVAILABLE

BIOMET 3i

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	29°	31.323.002.01-2	31.313.002.01-2
1,2	25°	22°	31.323.002.02-2	31.313.002.02-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,3	25°	20°	10°	31.323.002.21-2	31.313.002.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.101.01-2		
10	52.410.101.01-2	50.313.002.01-2	43.621.410.01-2 43.624.410.01-2
12	52.412.101.01-2		



LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.805.01-2	22.613.002.01-2	34.613.002.01-2
4	30°	33.490.805.01-2		
6		33.690.805.01-2		



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.002.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.084.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.003.01-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT


### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.002.01-2
2	42.303.002.02-2
3	42.303.002.03-2
4	42.303.002.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH 0003

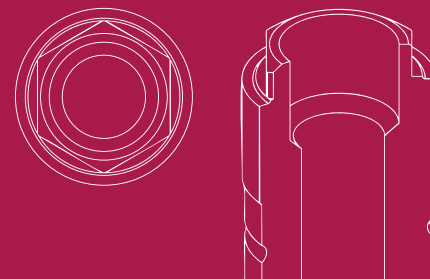

## LIST OF COMPATIBILITIES AVAILABLE

BIOMET 3i - BIOLOK - BTK - EASY IMPLANT - MICRODENT - MOZO-GRAU (TICARE) - SOUTHERN IMPLANTS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	30°	31.322.003.01-2	31.312.003.01-2
0,5	25°	30°	31.322.003.02-2	31.312.003.02-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1	30°	25°	15°	31.322.003.23-2	31.312.003.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.104.01-2	50.312.003.01-2	43.621.410.01-2
12	52.412.104.01-2		43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.716.01-2	22.612.003.01-2	34.612.003.01-2
4	25°	33.490.716.01-2		
6		33.690.716.01-2		



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.003.21-2	49.414.000.01-2	6	A	43.601.103.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.065.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.003.02-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH 0004



## LIST OF COMPATIBILITIES AVAILABLE

ASTRA - CORTEX - EASY IMPLANTS - EUROTEKNIKA - GALIMPLANT - IMPLANTSWISS - MOZO-GRAU (TICARE) - MPI - PROCLINIC  
REFLECT - SIGNO VINCES - SOUTHERN IMPLANTS - TITANIUM-FIX - UFIT - WARANTEC (ONEPLANT) - ZIACOM

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	45°	29°	31.323.004.01-2	31.313.004.01-2
2	30°	20°	31.323.004.02-2	31.313.004.02-2
3	25°	25°	31.323.004.03-2	31.313.004.03-2
4	20°	25°	31.323.004.04-2	31.313.004.04-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1	25°	20°	10°	31.323.004.21-2	31.313.004.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.313.004.01-2	43.621.410.01-2
12	52.412.103.01-2	50.313.004.03-2 (IG=3mm)	43.624.410.01-2



LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.004.02-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.754.01-2	22.613.004.01-2	34.613.004.01-2
4	25°	33.490.754.01-2		
6		33.690.754.01-2		



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.004.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.316.076.01-2	41.316.118.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.02-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.004.01-2
2	42.303.004.02-2
3	42.303.004.03-2
4	42.303.004.04-2

VIEW COMPONENTS




### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
2.5/3.9	48.312.004.02-2
3.5/4.9	48.312.004.03-2
4.5/5.9	48.312.004.04-2

VIEW COMPONENTS



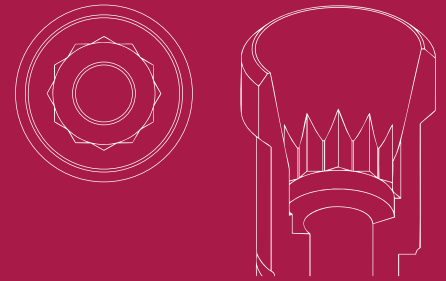

# COMPATIBLE WITH 0005

## LIST OF COMPATIBILITIES AVAILABLE

ASTRA - BIOGENESIS - CORTEX - GT MEDICAL - MOZO-GRAU (TICARE) - MPI - REFLECT - SIGNO VINCES - SOUTHERN IMPLANTS  
TITANIUM-FIX - UFIT

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	38°	23°	31.324.005.01-2	31.314.005.01-2
2	25°	15°	31.324.005.02-2	31.314.005.02-2
3	20°	-	31.324.005.03-2	31.314.005.03-2
4	15°	-	31.324.005.04-2	31.314.005.04-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH-5mm	$\alpha_s$ CH-7mm	$\alpha_s$ CH-9mm	NON ENGAGING	ENGAGING
1	25°	20°	10°	31.324.005.21-2	31.314.005.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.102.01-2	50.314.005.01-2	43.621.410.01-2
12	52.412.102.01-2	50.314.005.03-2 (IG=3mm)	43.624.410.01-2



#### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.958.01-2	22.614.005.01-2	34.614.005.01-2
4	30°	33.490.958.01-2		
6		33.690.958.01-2		



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.005.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



**SCREWS**

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.320.090.01-2	41.320.137.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.005.03-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH 0006

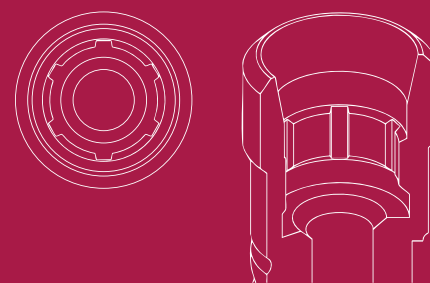

## LIST OF COMPATIBILITIES AVAILABLE

ASTRA

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	40°	20°	31.322.006.01-2	31.312.006.01-2
2	25°	12°	31.322.006.02-2	31.312.006.02-2
3	20°	30°	31.322.006.03-2	31.312.006.03-2
4	15°	30°	31.322.006.04-2	31.312.006.04-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,2	30°	20°	15°	31.322.006.21-2	31.312.006.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.105.01-2	50.312.006.03-2 (IG=3mm)	43.621.410.01-2
12	52.412.105.01-2		43.624.410.01-2



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.006.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.330.734.01-2	22.612.006.01-2	34.612.006.01-2
4	25°	33.430.734.01-2		
6		33.630.734.01-2		



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.006.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



**SCREWS**

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.316.072.01-2	41.316.115.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.01-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.006.01-2
2	42.302.006.02-2
3	42.302.006.03-2
4	42.302.006.04-2

VIEW COMPONENTS




### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
2.5/3.9	48.312.006.02-2
3.5/4.9	48.312.006.03-2
4.5/5.9	48.312.006.04-2

VIEW COMPONENTS



# COMPATIBLE WITH 0007



## LIST OF COMPATIBILITIES AVAILABLE

ASTRA

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	38°	17°	31.323.007.01-2	31.313.007.01-2
2	25°	12°	31.323.007.02-2	31.313.007.02-2
3	25°	-	31.323.007.03-2	31.313.007.03-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,5	25°	20°	10°	31.323.007.21-2	31.313.007.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.101.01-2		
10	52.410.101.01-2	50.313.007.01-2 50.313.007.03-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2
12	52.412.101.01-2		



LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.007.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.350.775.01-2	22.613.007.01-2	34.613.007.01-2
4	25°	33.450.775.01-2		
6		33.650.775.01-2		



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.007.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.318.074.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.005.02-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.007.01-2
2	42.303.007.02-2
3	42.303.007.03-2
4	42.303.007.04-2

VIEW COMPONENTS



### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
1.5/2.9	48.312.007.01-2
2.5/3.9	48.312.007.02-2
3.5/4.9	48.312.007.03-2


VIEW COMPONENTS



# COMPATIBLE WITH 0008

## LIST OF COMPATIBILITIES AVAILABLE

ASTRA

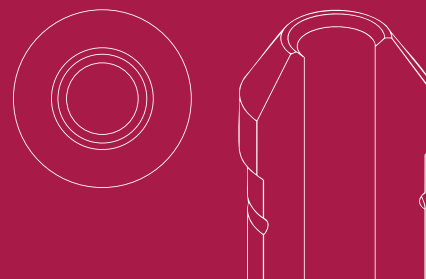

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	30°	31.323.008.01-2	-



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,5	25°	20°	10°	31.323.008.21-2	-



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.113.01-2	50.313.008.01-2	43.621.410.01-2 43.624.410.01-2



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.413.008.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.370.716.01-2
4	30°	33.470.716.01-2
6		33.670.716.01-2

### ANALOG

DIGITAL ANALOG
34.613.008.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

### SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.322.008.31-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		
	CAPS	HEIGHT	TYPE	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	




### SCREWS

DYNAMIC SCREW	LENTH	SCREWDRIVER
41.318.045.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2
STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.005.01-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH 0009

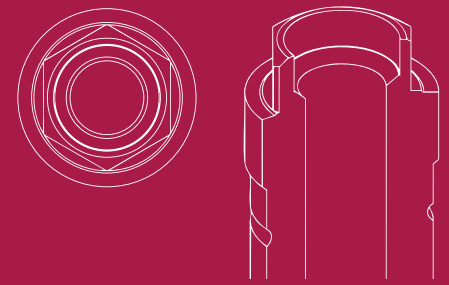

## LIST OF COMPATIBILITIES AVAILABLE

BTI - MPI - OSTEOPLUS - PROCLINIC


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	25°	31.322.009.01-2	31.312.009.01-2
0,5	25°	25°	31.322.009.02-2	31.312.009.02-2
1	25°	-	31.322.009.03-2	31.312.009.03-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.114.01-2	50.312.009.01-2	43.621.410.01-2
12	52.412.114.01-2		43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.716.01-2	22.612.009.01-2	34.612.009.01-2
4	25°	33.490.716.01-2		
6		33.690.716.01-2		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.320.065.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.008.01-2	Hex. 1.20	43.625.108.01-2



# COMPATIBLE WITH OO10

## LIST OF COMPATIBILITIES AVAILABLE

BTI



### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	29°	31.323.010.01-2	31.313.010.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.115.01-2	50.313.010.01-2	43.621.410.01-2
12	52.412.115.01-2	50.313.010.04-2 (IG=3mm)	43.624.410.012



#### LAB SCANBODY

30.413.002.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.716.01-2	22.613.010.01-2	34.613.010.01-2
4	30°	33.490.716.01-2		
6		33.690.716.01-2		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.065.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.003.01-2	Hex. 1.20	43.601.103.02-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.010.01-2
2	42.303.010.02-2
3	42.303.010.03-2
4	42.303.010.04-2


[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO11

## LIST OF COMPATIBILITIES AVAILABLE

CAMLOG

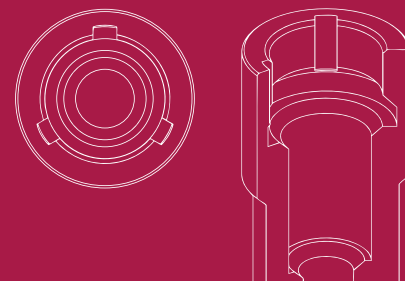

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	25°	29°	31.322.011.01-2	31.312.011.01-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,3	25°	25°	15°	-	31.312.011.21-2
2	25°	20°	15°	-	31.312.011.23-2
3	25°	20°	10°	-	31.312.011.24-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.108.01-2	50.312.011.01-2	43.621.410.01-2
12	52.412.108.01-2		43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

### DYNAMIC MILLING TOOL

### ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.804.01-2	34.612.011.01-2
4	20°	33.445.804.01-2	
6		33.645.804.01-2	



### SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.011.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.094.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2

STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.04-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT


GH (mm)	NON ENGAGING
1	42.302.011.01-2
2	42.302.011.02-2
3	42.302.011.03-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO12

LIST OF COMPATIBILITIES **AVAILABLE**  
CAMLOG

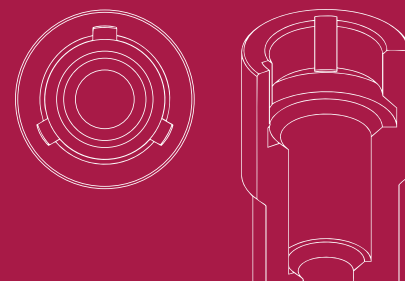

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	25°	30°	31.323.012.01-2	31.313.012.01-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH-5mm	$\alpha_s$ CH-7mm	$\alpha_s$ CH-9mm	NON ENGAGING	ENGAGING
0,3	25°	25°	15°	-	31.313.012.21-2
2	25°	20°	15°	-	31.313.012.23-2
3	25°	20°	10°	-	31.313.012.24-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.109.01-2	50.313.012.01-2	43.621.410.01-2
12	52.412.109.01-2		43.624.410.01-2



### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.804.01-2	34.613.012.01-2
4	20°	33.445.804.01-2	
6		33.645.804.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.012.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.094.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.04-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT


GH (mm)	NON ENGAGING
1	42.303.012.01-2
2	42.303.012.02-2
3	42.303.012.03-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH 0013

LIST OF COMPATIBILITIES **AVAILABLE**  
DIO IMPLANTS

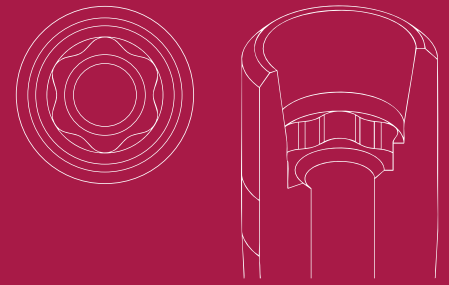

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,7	43°	23°	31.323.013.01-2	31.313.013.01-2
<b>LAB SCANBODY</b>				
30.413.002.01-2				



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.074.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.007.02-2	TORX T6	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

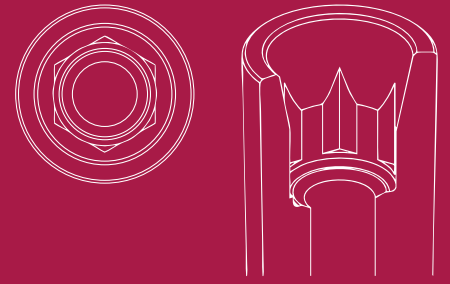

# COMPATIBLE WITH OO14

## LIST OF COMPATIBILITIES AVAILABLE

DENTIS - DIO IMPLANT - MEGAGEN

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
1,2	41°	23°	31.322.014.01-2	31.312.014.01-2
2	25°	17°	31.322.014.02-2	31.312.014.02-2
3	20°	25°	-	31.312.014.03-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_S$ CH=5mm	$\alpha_S$ CH=7mm	$\alpha_S$ CH=9mm	NON ENGAGING	ENGAGING
3	25°	20°	15°	31.322.014.23-2	31.312.014.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.128.01-2	50.312.014.03-2 (IG=3mm)	43.621.415.01-2



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.014.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.804.01-2	34.612.014.01-2
4	25°	33.445.804.01-2	
6		33.645.804.01-2	



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.014.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



**SCREWS**

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.314.067.01-2	41.314.105.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.003.04-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
2	42.302.014.02-2
3	42.302.014.03-2
4	42.302.014.04-2

VIEW COMPONENTS




### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
3.5/4.9	48.312.014.03-2
4.5/5.9	48.312.014.04-2

VIEW COMPONENTS



# COMPATIBLE WITH OO15

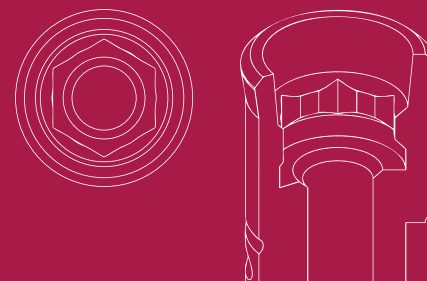

## LIST OF COMPATIBILITIES AVAILABLE

OXY - JDENTALCARE - MEGAGEN

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,7	43°	23°	31.323.015.01-2	31.313.015.01-2
2,5	25°	15°	31.323.015.02-2	31.313.015.02-2
3	25°	-	31.323.015.03-2	31.313.015.03-2
4	20°	-	31.323.015.04-2	31.313.015.04-2
5	15°	-	31.323.015.05-2	31.313.015.05-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1	30°	25°	20°	31.323.015.27-2	31.313.015.27-2
1,7	30°	25°	10°	31.323.015.21-2	31.313.015.21-2
2,5	25°	20°	10°	31.323.015.22-2	31.313.015.22-2
3,5	25°	20°	10°	-	31.313.015.26-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.104.01-2	50.313.015.01-2	43.621.410.01-2
12	52.412.104.01-2	50.313.015.03-2 (IG=3mm)	43.624.410.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.015.01-2



### DYNAMIC MILLING TOOL

### ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.805.01-2	34.613.015.01-2
4	25°	33.490.805.01-2	
6		33.690.805.01-2	



### SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.015.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.318.075.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.003.02-2	Hex. 1.20	43.601.103.02-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.015.01-2
2	42.303.015.02-2
3	42.303.015.03-2
4	42.303.015.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
1,5/2,9	48.312.015.01-2
2,5/3,9	48.312.015.02-2
4,5/5,9	48.312.015.04-2

[VIEW COMPONENTS](#)



### INTERNAL MULTI-UNIT


GH (mm)	ENGAGING
2	62.303.015.02-2
3	62.303.015.03-2
4	62.303.015.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH 0016

LIST OF COMPATIBILITIES **AVAILABLE**  
MIS

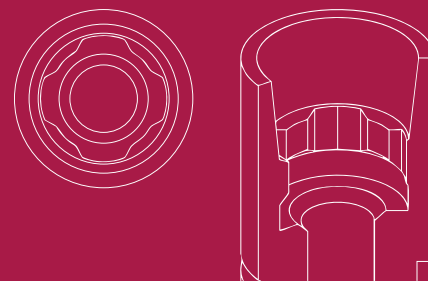

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,8	45°	28°	31.322.016.01-2	31.312.016.01-2
1,5	25°	25°	31.322.016.02-2	31.312.016.02-2




## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,5	25°	25°	15°	-	31.312.016.22-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.106.01-2		
10	52.410.106.01-2	50.312.016.01-2 50.312.016.04-2	43.621.410.01-2 43.624.410.01-2
12	52.412.106.01-2	(IG=3mm)	



### LAB SCANBODY

30.412.001.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL


## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.754.01-2	34.612.016.01-2
4	25°	33.460.754.01-2	
6		33.660.754.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.016.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		

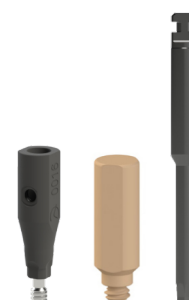

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.071.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2

STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.05-2	Hex. 1.27	43.625.105.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	ENGAGING
1	42.302.016.01-2
2	42.302.016.02-2
3	42.302.016.03-2
4	42.302.016.04-2

[VIEW COMPONENTS](#)




### ANGULATED MULTI-UNIT 20°

GH (mm)	NON ENGAGING
2.5/3.9	48.312.016.02-2
3.5/4.9	48.312.016.03-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO17

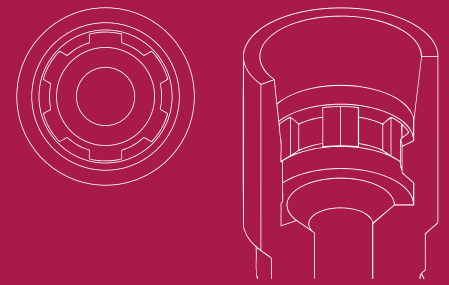

## LIST OF COMPATIBILITIES AVAILABLE MIS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,7	45°	24°	31.323.017.01-2	31.313.017.01-2
1,5	25°	15°	31.323.017.02-2	31.313.017.02-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,7	30°	25°	15°	31.323.017.21-2	31.313.017.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.101.01-2		
10	52.410.101.01-2	50.313.017.04-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2
12	52.412.101.01-2		



#### LAB SCANBODY

30.413.002.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.756.01-2	34.613.017.01-2
4	30°	33.460.756.01-2	
6		33.660.756.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.017.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.317.073.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.317.005.01-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	ENGAGING
2	42.303.017.02-2
<a href="#">VIEW COMPONENTS</a>	




### ANGULATED MULTI-UNIT 20°

GH (mm)	NON ENGAGING
2,5/3,9	48.312.017.02-2
3,5/4,9	48.312.017.03-2
<a href="#">VIEW COMPONENTS</a>	



# COMPATIBLE WITH OO18

LIST OF COMPATIBILITIES **AVAILABLE**  
MIS




## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	39°	18°	31.324.018.01-2	31.314.018.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.102.01-2	50.314.018.01-2	43.621.410.01-2
12	52.412.102.01-2		43.624.410.01-2




### LAB SCANBODY

30.413.002.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.756.01-2	34.614.018.01-2
4	30°	33.460.756.01-2	
6		33.660.756.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.317.073.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.317.005.01-2	Hex. 1.27	43.625.105.01-2



# COMPATIBLE WITH 0019

LIST OF COMPATIBILITIES **AVAILABLE**  
MIS




## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,8	45°	30°	31.322.019.01-2	31.312.019.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.105.01-2	50.312.019.01-2	43.621.410.01-2
12	52.412.105.01-2		43.624.410.01-2




### LAB SCANBODY

30.412.001.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.754.01-2	34.612.019.01-2
4	25°	33.460.754.01-2	
6		33.660.754.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.071.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.05-2	Hex. 1.27	43.625.105.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT


GH (mm)	ENGAGING
1	42.302.019.01-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO20

LIST OF COMPATIBILITIES **AVAILABLE**  
MIS



## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.323.020.01-2	-



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.112.01-2	50.313.020.01-2	43.620.411.01-2



### LAB SCANBODY

30.413.005.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.613.020.01-2
4	30°	33.490.716.01-2	
6		33.690.716.01-2	

## ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
54.322.020.31-2	49.416.000.04-2	13	D	43.625.105.01-2
	49.416.000.05-2	13	E	
	CAPS	HEIGHT	TYPE	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.044.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2

STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.06-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH OO21



## LIST OF COMPATIBILITIES AVAILABLE

ADIN - ALFA-GATE - BIONER - CONEXÃO SISTEMA DE PRÓTESE - HAHN IMPLANT (GLIDEWELL) - HI-TEC IMPLANT DIRECT - NOBEL BIO CARE - REFLECT - YOUSE IMPLANTS (SWEDEN & MARTINA GROUP)

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	43°	24°	31.322.021.01-2	31.312.021.01-2
2	25°	20°	31.322.021.02-2	31.312.021.02-2
3	20°	30°	31.322.021.03-2	31.312.021.03-2
4	15°	30°	31.322.021.04-2	31.312.021.04-2
5	15°	20°	31.322.021.05-2	31.312.021.05-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,5	25°	20°	10°	31.322.021.21-2	31.312.021.21-2
3	25°	20°	15°	31.322.021.23-2	31.312.021.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2		43.621.410.01-2
12	52.412.103.01-2	50.312.021.03-2 (IG=3mm)	43.624.410.01-2



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.021.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.335.754.01-2	22.612.021.01-2	34.612.021.01-2
4	25°	33.435.754.01-2		
6		33.635.754.01-2		



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.021.21-2	49.414.000.01-2	6	A	43.625.108.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.316.073.01-2	41.316.108.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.008.02-2	UNIGRIP	43.625.108.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.021.01-2
2	42.302.021.02-2
3	42.302.021.03-2
4	42.302.021.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	NON ENGAGING
1,5/2,9	48.312.021.01-2
2,5/3,9	48.312.021.02-2
4,5/5,9	48.312.021.04-2

[VIEW COMPONENTS](#)

### ANGULATED MULTI-UNIT 28°

GH (mm)	NON ENGAGING
3,5/5,4	48.612.021.03-2
4,5/6,4	48.612.021.04-2

[VIEW COMPONENTS](#)




### INTERNAL MULTI-UNIT

GH (mm)	ENGAGING
2	62.302.021.02-2
3	62.302.021.03-2
4	62.302.021.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH 0022

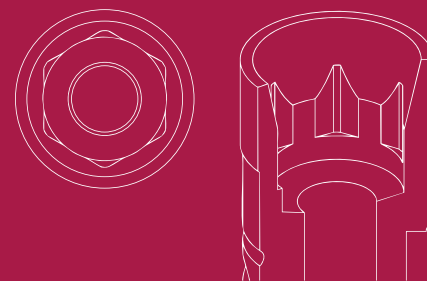

## LIST OF COMPATIBILITIES AVAILABLE

ADIN - ALFA-GATE - HAHN IMPLANT (GLIDEWELL) - HI-TEC - IMPLANT DIRECT - JDENTALCARE - NOBEL BIOCARE REFLECT - YOUSE IMPLANTS (SWEDEN & MARTINA GROUP)

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,3	40°	19°	31.323.022.01-2	31.313.022.01-2
2	25°	14°	31.323.022.02-2	31.313.022.02-2
3	20°	30°	31.323.022.03-2	31.313.022.03-2
4	15°	30°	31.323.022.04-2	31.313.022.04-2
5	15°	20°	31.323.022.05-2	31.313.022.05-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,3	30°	25°	10°	31.323.022.21-2	31.313.022.21-2
3	20°	20°	10°	31.323.022.23-2	31.313.022.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.101.01-2		
10	52.410.101.01-2	50.313.022.01-2 50.313.022.03-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2
12	52.412.101.01-2		



LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.022.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.335.758.01-2	22.613.022.01-2	34.613.022.01-2
4	30°	33.435.758.01-2		
6		33.635.758.01-2		



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
54.315.022.21-2	49.416.000.02-2	13	B	43.625.108.01-2
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



**SCREWS**

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
		18	43.618.201.01-2
41.320.075.01-2	41.320.117.01-2	24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.008.02-2	UNIGRIP	43.625.108.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_i$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.022.01-2
2	42.303.022.02-2
3	42.303.022.03-2
4	42.303.022.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	NON ENGAGING
1,5/2,9	48.312.022.01-2
2,5/3,9	48.312.022.02-2

[VIEW COMPONENTS](#)

### ANGULATED MULTI-UNIT 28°

GH (mm)	NON ENGAGING
3,5/5,4	48.612.022.03-2
4,5/6,4	48.612.022.04-2

[VIEW COMPONENTS](#)




### INTERNAL MULTI-UNIT

GH (mm)	ENGAGING
2	62.303.022.02-2
3	62.303.022.03-2
4	62.303.022.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO23



## LIST OF COMPATIBILITIES **AVAILABLE**

ACE - AVINENT - BIOGENESIS - BIOHORIZONS - DENTIS - DIO IMPLANTS - ELITE MEDICA - GT MEDICAL - KLOCKNER MEGAGEN - NEOBIOTECH - NOBEL BIO CARE - OSSTEM IMPLANT - RADHEX - STERI-OSS - TBR - TREE-OSS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	30°	31.322.023.01-2	31.312.023.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.312.023.01-2	43.621.410.01-2
12	52.412.103.01-2		43.624.410.01-2



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.023.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.805.01-2	22.612.023.01-2	34.612.023.01-2
4	25°	33.490.805.01-2		
6		33.690.805.01-2		



### ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

**SCREWS**


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.059.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.008.01-2	UNIGRIP	43.625.108.01-2



# COMPATIBLE WITH OO24

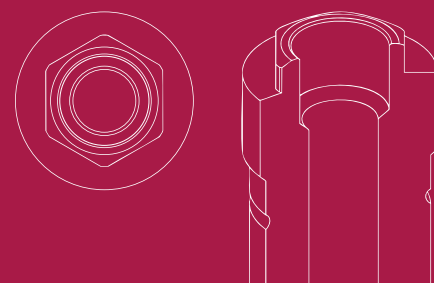

## LIST OF COMPATIBILITIES AVAILABLE

ACE - ANTHOGRYR - AVINENT - BIOGENESIS - B&W - BIOMET 3i - BIONER - BTI - BTK - DENTIS - DIO IMPLANTS - EASY IMPLANT - ECKERMANN  
 ELITE MEDICA - DSP BIOMEDICAL - EUROTEKNIKA - GALIMPLANT - GMI (ILERIMPLANT) - GT MEDICAL - INTRA-LOCK - KEYSTONE - KLOCKNER - LEADER - MEGAGEN  
 MICRODENT - MIS - MOZO-GRAU (TICARE) - MPI - NEODENT - NOBEL BIO CARE - NORMON - OSSTEM IMPLANT - OSTEOPLUS - OXY - PHIBO - PROCLINIC  
 RADHEX - SIGNO VINCES - SIN IMPLANTS - SOUTHERN IMPLANTS SOLUTIONS - STERNGOLD - SYTHEX - TREE-OSS - TRINON - ZIACOM

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	30°	31.323.024.01-2	31.313.024.01-2
0,5	30°	30°	31.323.024.02-2	31.313.024.02-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,3	30°	25°	10°	31.323.024.21-2	31.313.024.21-2
0,5	30°	25°	10°	31.323.024.22-2	31.313.024.22-2
1	30°	25°	10°	31.323.024.23-2	31.313.024.23-2
2	30°	25°	10°	31.323.024.24-2	31.313.024.24-2
3	25°	20°	15°	31.323.024.25-2	31.313.024.25-2
4	25°	20°	15°	31.323.024.26-2	31.313.024.26-2



LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.024.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.390.716.01-2
4	30°	33.490.716.01-2
6		33.690.716.01-2

## ANALOG

ANALOG	DIGITAL ANALOG
22.613.024.01-2	34.613.024.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.024.21-2	49.414.000.01-2	6	A	43.625.108.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.060.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.008.01-2	UNIGRIP	43.625.108.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT


GH (mm)	NON ENGAGING
2	42.303.024.02-2
3	42.303.024.03-2

[VIEW COMPONENTS](#)



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm G1 = Standard maximum angulation G2 = Standard maximum angulation G3 = Direct to implant maximum angulation

# COMPATIBLE WITH OO25

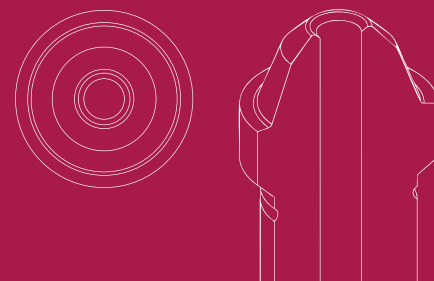

## LIST OF COMPATIBILITIES AVAILABLE

AB - ACE - ADIN - AVINENT - BIOHORIZONS - BIOMET 3i - BIONER - CORTEX - DENTIS - EASY IMPLANT - EUROTEKNIKA - GALIMPLANT - GMI (ILERIMPLANT) - HAHN IMPLANT (GLIDEWELL) - IMPLANTSWISS - JDENTALCARE - MEDENTIS - MEDENTIKA - MEGAGEN - MONOIMPLANT - NEOBIOTECH - NEODENT - NOBEL BIO CARE - OSSTEM IMPLANT - SEWON MEDIX - SIN IMPLANTS - SOUTHERN IMPLANTS - TREE-OSS - WIN

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	30°	31.323.025.01-2	-




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,3	30°	25°	10°	31.323.025.21-2	-



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.112.01-2	50.313.025.02-2	43.620.411.01-2 43.621.410.01-2
10	52.410.111.01-2	50.313.025.01-2	43.624.410.01-2



LAB SCANBODY	MINI SCANBODY	SCANALOG
30.413.005.01-2	53.413.025.01-2	23.413.025.01-2 23.313.025.01-2 (Titanium)




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.716.01-2	22.613.025.01-2	34.613.025.01-2
4	30°	33.490.716.01-2		
6		33.690.716.01-2		



**SCANBODY REFERENCE**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
54.322.025.31-2	49.416.000.04-2	13	D	43.625.108.01-2
	49.416.000.05-2	13	E	
	<b>CAPS</b>	<b>HEIGHT</b>	<b>TYPE</b>	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_i$  = Direct to implant maximum angulation

SCREWS


DYNAMIC SCREW	DYNAMIC SCREW Ø2,6	LENGTH	SCREWDRIVER
		18	43.618.201.01-2
41.314.039.01-2	41.314.050.31-2 (Temporary or Zirconio Direct MU)	24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.008.01-2	UNIGRIP	43.625.108.01-2



# COMPATIBLE WITH OO26

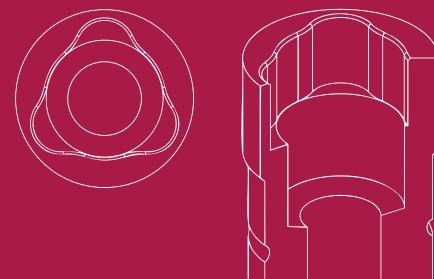


## LIST OF COMPATIBILITIES AVAILABLE

ACE - IMPLANT DIRECT - NOBEL BIOCARE - SOUTHERN IMPLANTS - TREE-OSS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	29°	31.322.026.01-2	31.312.026.01-2
1,2	25°	22°	31.322.026.02-2	31.312.026.02-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,5	25°	20°	10°	31.322.026.21-2	31.312.026.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.108.01-2	50.312.026.04-2 (IG=3mm)	43.621.410.01-2
12	52.412.108.01-2		43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.805.01-2	22.612.026.01-2	34.612.026.01-2
4	25°	33.490.805.01-2		
6		33.690.805.01-2		



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
54.315.026.21-2	49.416.000.02-2	13	B	43.625.108.01-2
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.075.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.008.01-2	UNIGRIP	43.625.108.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH OO27



## LIST OF COMPATIBILITIES AVAILABLE

ACE - IMPLANT DIRECT - NOBEL BIOCARE - SOUTHERN IMPLANTS - TREE-OSS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	35°	29°	31.323.027.01-2	31.313.027.01-2
1,2	25°	22°	31.323.027.02-2	31.313.027.02-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,3	25°	20°	10°	31.323.027.21-2	31.313.027.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.109.01-2	50.313.027.01-2	43.621.410.01-2
12	52.412.109.01-2		43.624.410.01-2



#### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.958.01-2	22.613.027.01-2	34.613.027.01-2
4	30°	33.490.958.01-2		
6		33.690.958.01-2		



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
54.315.027.21-2	49.416.000.02-2	13	B	43.625.108.01-2
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.320.090.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.008.03-2	UNIGRIP	43.625.108.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

# COMPATIBLE WITH OO28



## LIST OF COMPATIBILITIES **AVAILABLE**

ACE - IMPLANT DIRECT - NOBEL BIOCARE - SOUTHERN IMPLANTS - TREE-OSS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	35°	30°	31.324.028.01-2	31.314.028.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.109.01-2	50.314.028.01-2	43.621.410.01-2
12	52.412.109.01-2		43.624.410.01-2



#### LAB SCANBODY

30.413.002.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3	30°	33.390.958.01-2	22.614.028.01-2	34.614.028.01-2
4		33.490.958.01-2		
6		33.690.958.01-2		



### ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.028.21-2	49.414.000.01-2	6	A	43.625.108.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.090.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.008.03-2	UNIGRIP	43.625.108.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm G<sub>s</sub> = Standard maximum angulation G<sub>c</sub> = Standard maximum angulation G<sub>d</sub> = Direct to implant maximum angulation

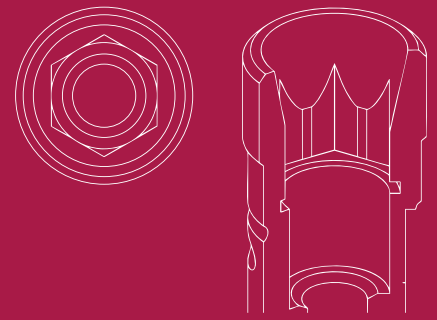

# COMPATIBLE WITH OO29

## LIST OF COMPATIBILITIES AVAILABLE

BIOCONCEPT - BTK - HIOSSEN - NEOBIOTECH - OSSTEM IMPLANT - SEWON MEDIX

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	30°	23°	31.322.029.01-2	31.312.029.01-2
2	25°	15°	31.322.029.02-2	31.312.029.02-2
3	20°	25°	31.322.029.03-2	31.312.029.03-2
4	15°	25°	31.322.029.04-2	31.312.029.04-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,2	25°	20°	20°	31.322.029.21-2	31.312.029.21-2
2	25°	20°	15°	-	31.312.029.22-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.312.029.01-2	43.621.410.01-2
12	52.412.103.01-2	50.312.029.03-2 (IG=3mm)	43.624.410.01-2



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.029.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

### DYNAMIC MILLING TOOL

### ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.804.01-2	34.613.029.01-2
4	20°	33.445.804.01-2	
6		33.645.804.01-2	



### SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.029.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



### SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.316.094.01-2	41.316.132.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.003.02-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_i$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.029.01-2
2	42.302.029.02-2
3	42.302.029.03-2
4	42.302.029.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	NON ENGAGING
2,5/3,9	48.312.029.02-2
3,5/4,9	48.312.029.03-2
4,5/5,9	48.312.029.04-2

[VIEW COMPONENTS](#)



### INTERNAL MULTI-UNIT

GH (mm)	ENGAGING
2	62.302.029.02-2
4	62.302.029.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO30




## LIST OF COMPATIBILITIES AVAILABLE

BIOCONCEPT - BIOTEM - COWELLMEDI - DENTEM - DENTIS - DENTIUM - DIO IMPLANTS - EASY IMPLANT  
F&B IMPLANT (FIT & BRILLIANT) - HIOSSEN - IBS - IDO IMPLANTS - IMPLANTSWISS - KUWOTECH - MEGAGEN  
NEOBIOTECH - OSSTEM IMPLANT - POINT IMPLANT - SEWON MEDIX - STARK IMPLANTS - YES IMPLANT

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
1,1	42°	25°	31.323.030.01-2	31.313.030.01-2
2	25°	15°	31.323.030.02-2	31.313.030.02-2
3	20°	30°	31.323.030.03-2	31.313.030.03-2
4	15°	30°	31.323.030.04-2	31.313.030.04-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_S$ CH=5mm	$\alpha_S$ CH=7mm	$\alpha_S$ CH=9mm	NON ENGAGING	ENGAGING
1,1	25°	20°	10°	31.323.030.21-2	31.313.030.21-2
2	25°	20°	15°	31.323.030.22-2	31.313.030.22-2
3	25°	20°	10°	31.323.030.23-2	31.313.030.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.101.01-2		
10	52.410.101.01-2	50.313.030.01-2 50.313.030.03-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2
12	52.412.101.01-2		



LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.030.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.808.01-2	34.613.030.01-2
4	30°	33.445.808.01-2	
6		33.645.808.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.030.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



## SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.320.079.01-2	41.320.125.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.003.04-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.030.01-2
2	42.303.030.02-2
3	42.303.030.03-2
4	42.303.030.04-2
5	42.303.030.05-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
1,5/2,9	48.312.030.01-2
2,5/3,9	48.312.030.02-2
3,5/4,9	48.312.030.03-2
4,5/5,9	48.312.030.04-2

[VIEW COMPONENTS](#)




### INTERNAL MULTI-UNIT

GH (mm)	ENGAGING
2	62.303.030.02-2
3	62.303.030.03-2
4	62.303.030.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH 0033

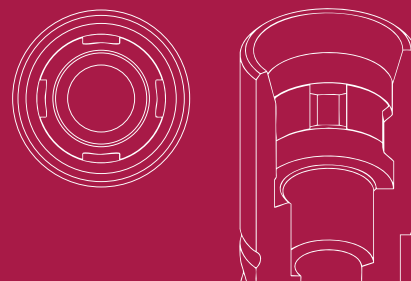

## LIST OF COMPATIBILITIES AVAILABLE

BIOCONCEPT - IHDE DENTAL (IMBIODENT) - STRAUMANN

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,3	38°	18°	31.322.033.01-2	31.312.033.01-2
2	20°	14°	31.322.033.02-2	31.312.033.02-2
3	15°	25°	31.322.033.03-2	31.312.033.03-2
4	15°	25°	31.322.033.04-2	31.312.033.04-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,3	25°	20°	10°	31.322.033.21-2	31.312.033.21-2
3	20°	15°	10°	31.322.033.23-2	31.312.033.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREW/DRIVER ADAPTOR
8	52.408.106.01-2		
10	52.410.106.01-2	50.312.033.03-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2
12	52.412.106.01-2		



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.033.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.315.804.01-2	22.612.033.01-2	34.612.033.01-2
4	25°	33.415.804.01-2		
6		33.615.804.01-2		



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.033.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.316.078.01-2	41.316.124.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.01-2	TORX T6	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_i$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.033.01-2
2	42.302.033.02-2
3	42.302.033.03-2
4	42.302.033.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
2,5/3,9	48.312.033.02-2
3,5/4,9	48.312.033.03-2
4,5/5,9	48.312.033.04-2

[VIEW COMPONENTS](#)



### INTERNAL MULTI-UNIT

GH (mm)	ENGAGING
4	62.302.033.04-2


[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO35

## LIST OF COMPATIBILITIES AVAILABLE

BIOCONCEPT - IHDE DENTAL (IMBIODENT) - STRAUMANN

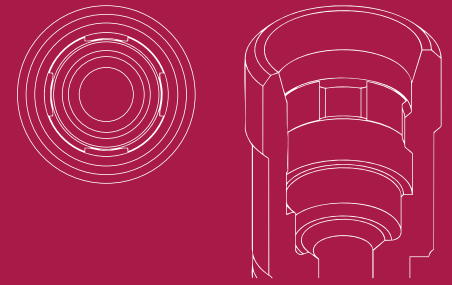

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,1	39°	18°	31.323.035.01-2	31.313.035.01-2
2	20°	14°	31.323.035.02-2	31.313.035.02-2
3	15°	30°	31.323.035.03-2	31.313.035.03-2
4	15°	30°	31.323.035.04-2	31.313.035.04-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=5mm	$\alpha_s$ CH=5mm	NON ENGAGING	ENGAGING
1,1	25°	20°	10°	31.323.035.21-2	31.313.035.21-2
3	20°	15°	10°	31.323.035.23-2	31.313.035.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.107.01-2	50.313.035.01-2	43.621.410.01-2
12	52.412.107.01-2	50.313.035.03-2 (IG=3mm)	43.624.410.01-2



LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.035.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.315.804.01-2	22.613.035.01-2	34.613.035.01-2
4	25°	33.415.804.01-2		
6		33.615.804.01-2		



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.035.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.316.078.01-2	41.316.124.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.01-2	TORX T6	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm G<sub>s</sub> = Standard maximum angulation G<sub>d</sub> = Standard maximum angulation G<sub>d</sub> = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.035.01-2
2	42.303.035.02-2
3	42.303.035.03-2
4	42.303.035.04-2

VIEW COMPONENTS




### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
2,5/3,9	48.312.035.02-2
3,5/4,9	48.312.035.03-2

VIEW COMPONENTS



# COMPATIBLE WITH OO37

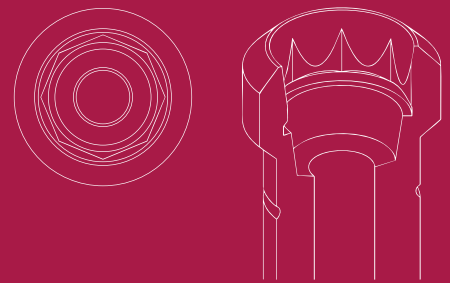

## LIST OF COMPATIBILITIES AVAILABLE

ACE - ANTHOGRYR - BIOCONCEPT - BIOGENESIS - DENTIS - DENTIUM - EUROTEKNIKA - GT MEDICAL - IMPLANT DIRECT  
MEGAGEN - PROCLINIC - SOUTHERN IMPLANTS - STRAUMANN - TRINON - ZIMMER


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	25°	31.323.037.01-2	31.313.037.01-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,6	30°	25°	15°	31.323.037.21-2	31.313.037.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.110.01-2		
10	52.410.110.01-2	50.313.037.04-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2
12	52.412.110.01-2		



LAB SCANBODY	SCANALOG
30.413.004.01-2	23.413.037.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.315.708.01-2	22.613.037.01-2	34.613.037.01-2
4	30°	33.415.708.01-2		
6		33.615.708.01-2		



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.037.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.067.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.007.01-2	TORX T6	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.037.01-2


[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO38

## LIST OF COMPATIBILITIES AVAILABLE

XIVE

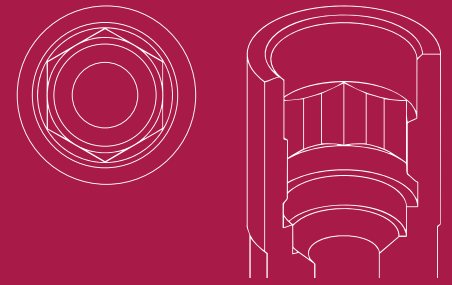

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,7	45°	29°	31.322.038.01-2	31.312.038.01-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,7	30°	25°	10°	31.322.038.21-2	31.312.038.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.312.038.01-2	43.621.410.01-2
12	52.412.103.01-2		43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.804.01-2	34.612.038.01-2
4	25°	33.445.804.01-2	
6		33.645.804.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.081.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.004.02-2	Hex. 1.25	43.601.104.01-2



# COMPATIBLE WITH 0039

LIST OF COMPATIBILITIES **AVAILABLE**  
SIN IMPLANTS - XIVE

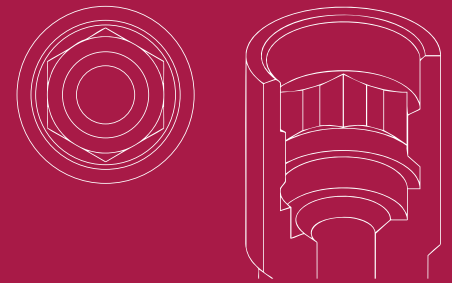

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,7	45°	29°	31.323.039.01-2	31.313.039.01-2
2	25°	-	31.323.039.03-2	31.313.039.03-2




## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,7	30°	25°	10°	31.323.039.21-2	31.313.039.21-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.114.01-2	50.313.039.01-2	43.621.410.01-2
12	52.412.114.01-2		43.624.410.01-2



### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2	34.613.039.01-2
4	25°	33.445.856.01-2	
6		33.645.856.01-2	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.081.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.004.02-2	Hex. 1.25	43.601.104.01-2



## MULTI-UNIT


### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.039.01-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO40



## LIST OF COMPATIBILITIES AVAILABLE

AB - ACE - ADIN - ALFA-GATE - ALPHABIO - ANCLADEN - ARDS - BIOHORIZONS - BIONER - BIOTEC - BTK - B&W - CORTEX - DITRON  
DMI DENTAL SUPPLY - HI-TEC - IMPLANT DIRECT - IMPLANT GENESIS - INTRA-LOCK - JDENTALCARE - LEADER - MIS - NORIS MEDICAL  
OSTEOPLUS - PROCLINIC - REFLECT - SOUTHERN IMPLANTS - TREE-OSS - TRI DENTAL IMPLANTS - VULKAN IMPLANTS - ZIMMER

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.322.040.01-2	31.312.040.01-2 31.312.042.01-2 (Friction Fit)
1,5	25°	25°	31.322.040.02-2	31.312.040.02-2
3	20°	30°	31.322.040.03-2	31.312.040.03-2
4	15°	30°	31.322.040.04-2	31.312.040.04-2
5	10°	23°	31.322.040.05-2	31.312.040.05-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,6	30°	25°	20°	31.322.040.21-2	31.312.040.21-2
1	30°	25°	20°	31.322.040.29-2	31.312.040.29-2
2	25°	20°	15°	-	31.312.040.28-2
3	25°	20°	15°	31.322.040.23-2	31.312.040.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.101.01-2		
10	52.410.101.01-2	50.312.040.03-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2
12	52.412.101.01-2		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.040.01-2



**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.370.716.01-2	22.612.040.01-2	34.612.040.01-2
4	25°	33.470.716.01-2		
6		33.670.716.01-2		



**SCANBODY OP**

SCANBODY	PEEK	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
54.315.040.21-2	49.416.000.02-2	13	B	43.625.105.01-2
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



**SCREWS**

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
		18	43.618.201.01-2
41.317.071.01-2	41.317.106.01-2	24	43.624.201.01-2
		32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

STRAIGHT SCREW	TYPE	SCREWDRIVER
40.317.004.01-2	Hex. 1.27	43.601.104.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.040.01-2
2	42.302.040.02-2
3	42.302.040.03-2
4	42.302.040.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
2.5/3.9	48.312.040.02-2
3.5/4.9	48.312.040.03-2
4.5/5.9	48.312.040.04-2

[VIEW COMPONENTS](#)




### INTERNAL MULTI-UNIT

GH (mm)	NON ENGAGING
4	62.302.040.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO4OB

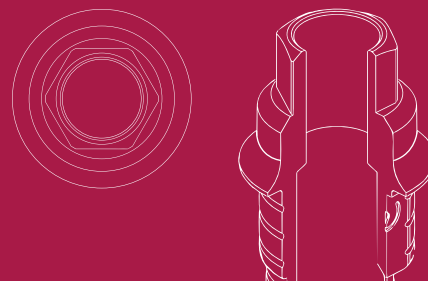

## LIST OF COMPATIBILITIES AVAILABLE

AVINENT - ECKERMANN - GMI (ILERIMPLANT) - MICRODENT - NORMON - NOVA IMPLANTS - PALTOP - RADHEX - RITTER WIN - ZIACOM

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.322.040.01-2	31.312.040.01-2 31.312.042.01-2 (Friction Fit)
1,5	25°	25°	31.322.040.02-2	31.312.040.02-2
3	20°	30°	31.322.040.03-2	31.312.040.03-2
4	15°	30°	31.322.040.04-2	31.312.040.04-2
5	10°	23°	31.322.040.05-2	31.312.040.05-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_S$ CH=5mm	$\alpha_S$ CH=7mm	$\alpha_S$ CH=9mm	NON ENGAGING	ENGAGING
0,6	30°	25°	20°	31.322.040.21-2	31.312.040.21-2
1	30°	25°	20°	31.322.040.29-2	31.312.040.29-2
2	25°	20°	15°	-	31.312.040.28-2
3	25°	20°	15°	31.322.040.23-2	31.312.040.23-2



### LAB SCANBODY

30.412.001.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.071.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH OO41

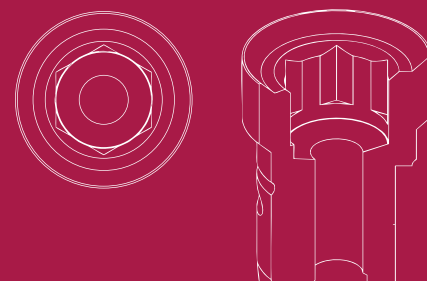

## LIST OF COMPATIBILITIES AVAILABLE

ACE - BIOHORIZONS - BIONER - DENTAL TECH - HI-TEC - IMPLANT DIRECT - INTRA-LOCK - MISS - PALTOP - REFLECT ZIMMER

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,4	45°	30°	31.323.041.01-2	31.323.041.02-2 31.313.043.01-2 (Friction Fit)
1,5	30°	25°	31.323.041.02-2	31.313.041.02-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,4	30°	20°	10°	31.323.041.21-2	31.313.041.21-2
1,5	30°	25°	15°	31.323.041.22-2	31.313.041.22-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.102.01-2	50.313.041.01-2	43.621.410.01-2
12	52.412.102.01-2	50.313.041.03-2 (IG=3mm)	43.624.410.01-2



LAB SCANBODY	SCANALOG
30.413.002.01-2	23.413.041.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.370.716.01-2	22.613.041.01-2	34.613.041.01-2
4	30°	33.470.716.01-2		
6		33.670.716.01-2		



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.041.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



**SCREWS**

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.317.071.01-2	41.317.106.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.317.004.01-2	Hex. 1.27	43.601.104.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT


### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.041.01-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO41B

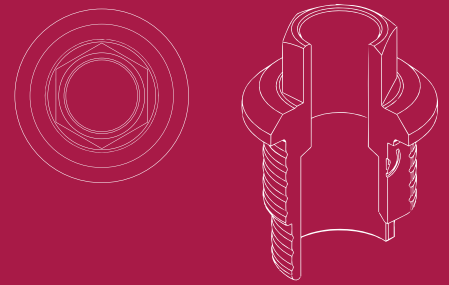

## LIST OF COMPATIBILITIES AVAILABLE

ECKERMANN - DENTEGRIS - GMI (ILERIMPLANT) - RADHEX

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,4	45°	30°	31.323.041.01-2	31.313.041.01-2
1,5	30°	25°	31.323.041.02-2	31.313.041.02-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,4	30°	20°	10°	31.323.041.21-2	31.313.041.21-2
1,5	30°	25°	15°	31.323.041.22-2	31.313.041.22-2



### LAB SCANBODY

30.413.002.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.370.716.01-2
4	30°	33.470.716.01-2
6		33.670.716.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.071.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH OO44



## LIST OF COMPATIBILITIES AVAILABLE KEYSTONE

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	42°	23°	31.322.044.01-2	31.312.044.01-2
2	25°	-	31.322.044.02-2	31.312.044.02-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1	25°	20°	10°	31.322.044.21-2	31.312.044.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.105.01-2	50.312.044.01-2	43.621.410.01-2
12	52.412.105.01-2		43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.612.044.01-2
4	25°	33.490.716.01-2	
6		33.690.716.01-2	



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.065.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.003.01-2	Hex. 1.20	43.601.103.02-2



# COMPATIBLE WITH OO45



## LIST OF COMPATIBILITIES AVAILABLE KEYSTONE

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	43°	22°	31.323.045.01-2	31.313.045.01-2
2	25°	-	31.323.045.02-2	31.313.045.02-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1	25°	20°	10°	31.323.045.21-2	31.313.045.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.118.01-2	50.313.045.01-2	43.621.410.01-2
12	52.412.118.01-2		43.624.410.01-2



#### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.613.045.01-2
4	30°	33.490.716.01-2	
6		33.690.716.01-2	



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.065.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.003.01-2	Hex. 1.20	43.601.103.02-2



# COMPATIBLE WITH OO46



## LIST OF COMPATIBILITIES AVAILABLE KEYSTONE

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	42°	21°	31.324.046.01-2	31.314.046.01-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1	30°	20°	10°	31.324.046.21-2	31.314.046.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.125.01-2	50.314.046.01-2	43.621.410.01-2 43.624.410.01-2



#### LAB SCANBODY

30.413.002.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.614.046.01-2
4	30°	33.490.716.01-2	
6		33.690.716.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.065.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.003.01-2	Hex. 1.20	43.601.103.02-2



# COMPATIBLE WITH OO47

LIST OF COMPATIBILITIES **AVAILABLE**  
NEOSS



## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.322.047.01-2	31.312.047.01-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_S$ CH=5mm	$\alpha_S$ CH=7mm	$\alpha_S$ CH=9mm	NON ENGAGING	ENGAGING
0,6	30°	25°	20°	-	31.312.047.21-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
9	52.409.123.01-2		
10	52.410.123.01-2	50.312.047.01-2	43.621.410.01-2 43.624.410.01-2
12	52.412.123.01-2		



### LAB SCANBODY

30.412.001.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.612.047.01-2
4	25°	33.490.716.01-2	
6		33.690.716.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.047.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.074.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.007.02-2	TORX T6	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH OO48

LIST OF COMPATIBILITIES **AVAILABLE**  
NEOSS



## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.323.048.01-2	31.313.048.01-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_S$ CH=5mm	$\alpha_S$ CH=7mm	$\alpha_S$ CH=9mm	NON ENGAGING	ENGAGING
0,6	30°	25°	20°	31.323.048.21-2	31.313.048.21-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
9	52.409.123.01-2		
10	52.410.123.01-2	50.312.047.01-2	43.621.410.01-2 43.624.410.01-2
12	52.412.123.01-2		



### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.612.047.01-2
4	30°	33.490.716.01-2	
6		33.690.716.01-2	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.320.074.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.007.02-2	TORX T6	43.601.107.01-2



# COMPATIBLE WITH OO49

## LIST OF COMPATIBILITIES AVAILABLE

BEGO

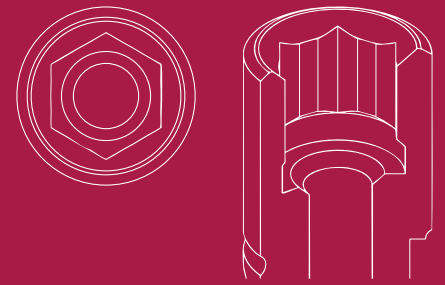


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.321.049.01-2	31.311.049.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.116.01-2		43.621.410.01-2
12	52.412.116.01-2	50.311.049.01-2	43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.325.472.01-2*	34.611.049.01-2
4	25°	33.425.472.01-2*	
6		33.625.472.01-2*	



\* Only for titanium and soft materials

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.064.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.004.01-2	Hex. 1.25	43.601.104.01-2



# COMPATIBLE WITH OO50

LIST OF COMPATIBILITIES **AVAILABLE**  
BEGO

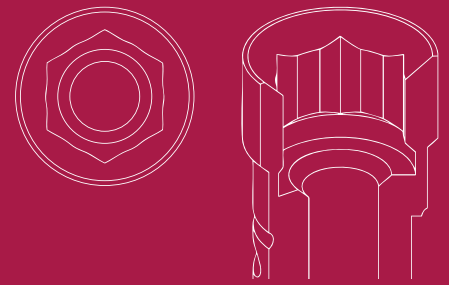

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	27°	31.323.051.01-2	31.313.051.01-2
2	25°	-	31.323.051.03-2	31.313.051.03-2




## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
2	25°	20°	15°	31.323.051.23-2	31.313.051.23-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.117.01-2		43.621.410.01-2
12	52.412.117.01-2	50.312.050.04-2 (IG=3mm)	43.624.410.01-2



### LAB SCANBODY

30.412.001.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.335.676.01-2	34.612.050.01-2
4	25°	33.435.676.01-2	
6		33.635.676.01-2	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.064.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.004.03-2	Hex. 1.25	43.601.104.01-2



## MULTI-UNIT


### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.050.01-2
2	42.302.050.02-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO51



## LIST OF COMPATIBILITIES AVAILABLE

BEGO

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	25°	31.323.051.01-2	31.313.051.01-2
2	25°	-	31.323.051.03-2	31.313.051.03-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
2	25°	20°	15°	31.323.051.23-2	31.313.051.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.118.01-2	50.313.051.01-2	43.621.410.01-2
12	52.412.118.01-2	50.313.051.04-2 (IG=3mm)	43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.335.676.01-2	34.613.051.01-2
4	25°	33.435.676.01-2	
6		33.635.676.01-2	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.064.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.004.03-2	Hex. 1.25	43.601.104.01-2



# COMPATIBLE WITH OO52

## LIST OF COMPATIBILITIES AVAILABLE

BEGO

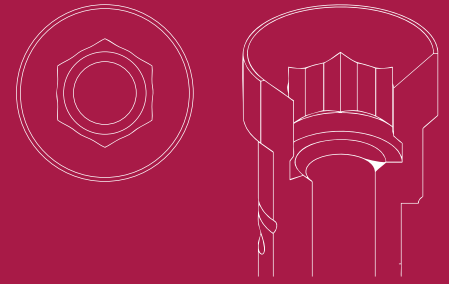

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	27°	31.324.052.01-2	31.314.052.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.102.01-2		43.621.410.01-2
12	52.412.102.01-2	50.314.052.04-2 (IG=3mm)	43.624.410.01-2



#### LAB SCANBODY


30.413.002.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.335.676.01-2	34.614.052.01-2
4	30°	33.435.676.01-2	
6		33.635.676.01-2	

### ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.064.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.004.03-2	Hex. 1.25	43.601.104.01-2



# COMPATIBLE WITH OO54

LIST OF COMPATIBILITIES **AVAILABLE**  
KLOCKNER

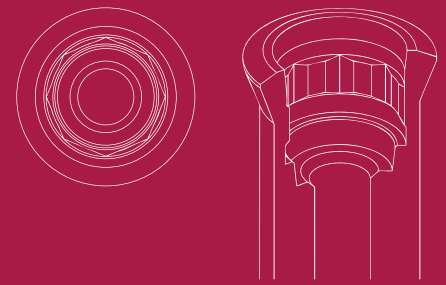


## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	25°	31.323.054.01-2	31.313.054.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.119.01-2		43.621.410.01-2
12	52.412.119.01-2	50.314.054.01-2	43.624.410.01-2



### LAB SCANBODY

30.413.002.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2	34.614.054.01-2
4	30°	33.445.856.01-2	
6		33.645.856.01-2	



## ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.318.067.01-2	18	43.618.201.01-2
41.318.051.02-2 (OCTACONE 12° & PILAR 25°)	24	43.624.201.01-2
	32	43.632.201.01-2



## STRAIGHT SCREW


40.318.012.01-2



# COMPATIBLE WITH OO57

## LIST OF COMPATIBILITIES AVAILABLE

BIOMET 3i

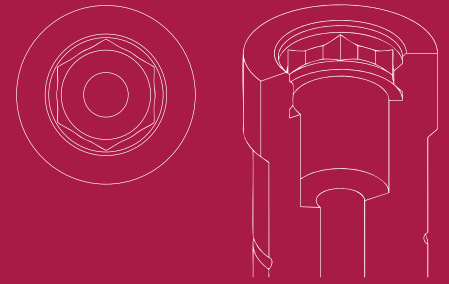


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	27°	31.324.057.01-2	31.314.057.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.101.01-2		
10	52.410.101.01-2	50.314.057.01-2	43.621.410.01-2 43.624.410.01-2
12	52.412.101.01-2		



#### LAB SCANBODY

30.414.003.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.805.01-2	22.614.057.01-2	34.614.057.01-2
4	30°	33.490.805.01-2		
6		33.690.805.01-2		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.084.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.003.01-2	Hex. 1.20	43.601.103.02-2



# COMPATIBLE WITH OO58

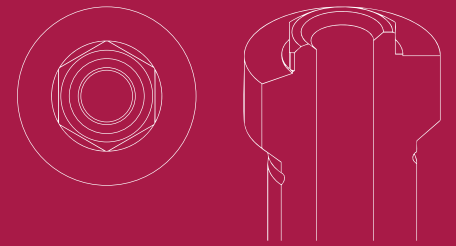

## LIST OF COMPATIBILITIES **AVAILABLE**

ACE - ANTHOGRYR - B&W - BIOGENESIS - BIOMET 3i - BIONER - EASY IMPLANT - LEADER - MEGAGEN - MICRODENT  
MIS - MPI - OSSTEM IMPLANT - PROCLINIC - SIN IMPLANTS - SOUTHERN IMPLANTS - TBR

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	30°	31.324.058.01-2	31.314.058.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.118.01-2	50.314.058.01-2	43.621.410.01-2
12	52.412.118.01-2		43.624.410.01-2



#### LAB SCANBODY

30.414.003.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3	30°	33.390.716.01-2	22.614.058.01-2	34.614.058.01-2
4		33.490.716.01-2		
6		33.690.716.01-2		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.320.047.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.003.02-2	Hex. 1.20	43.601.103.02-2



# COMPATIBLE WITH 0059




## LIST OF COMPATIBILITIES AVAILABLE

BTI

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,7	45°	27°	31.324.059.01-2	31.314.059.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.115.01-2	50.313.010.01-2	43.621.410.01-2
12	52.412.115.01-2	50.313.010.04-2 (IG=3mm)	43.624.410.01-2




#### LAB SCANBODY

30.414.003.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG
3		33.390.716.01-2	22.614.059.01-2
4	30°	33.490.716.01-2	
6		33.690.716.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.065.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.003.01-2	Hex. 1.20	43.601.103.02-2



# COMPATIBLE WITH OO60

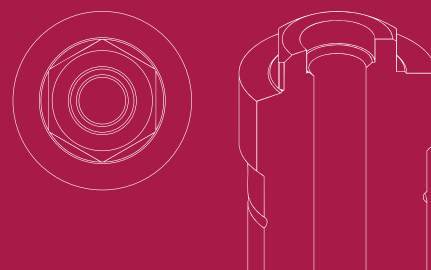

## LIST OF COMPATIBILITIES AVAILABLE

BTI

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	30°	31.324.060.01-2	31.314.060.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.122.01-2	50.314.060.01-2	43.621.410.01-2 43.624.410.01-2



#### LAB SCANBODY

30.415.007.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.716.01-2	22.614.060.01-2	34.614.060.01-2
4	30°	33.490.716.01-2		
6		33.690.716.01-2		



### ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.320.060.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.003.02-2	Hex. 1.20	43.601.103.02-2



# COMPATIBLE WITH OO61

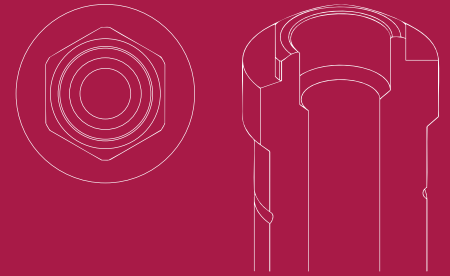

## LIST OF COMPATIBILITIES **AVAILABLE**

AVINENT - COWELLMEDI - DENTIS - DIO IMPLANTS - ELITE MEDICA - GMI (ILERIMPLANT) - GT MEDICAL - KEYSTONE  
KLOCKNER - MOZO-GRAU (TICARE) - NOBEL BIOCARE - OSSTEM IMPLANT - TREE-OSS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.324.061.01-2	31.314.061.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.125.01-2	50.314.061.01-2	43.621.410.01-2 43.624.410.01-2



#### LAB SCANBODY

30.415.007.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.390.958.01-2	22.614.061.01-2	34.614.061.01 -2
4	30°	33.490.958.01-2		
6		33.690.958.01-2		



### ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.325.067.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.325.008.01-2	UNIGRIP	43.625.108.01-2



# COMPATIBLE WITH OO66

LIST OF COMPATIBILITIES **AVAILABLE**  
ASTRA

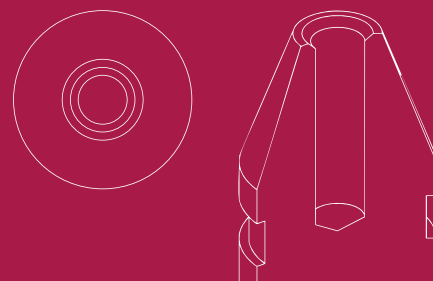

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.323.066.01-2	-



### LAB SCANBODY

30.412.001.01-2



## ANALOG

### ANALOG

22.613.066.01-2



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.039.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.008.01-2	UNIGRIP	43.625.108.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH OO74

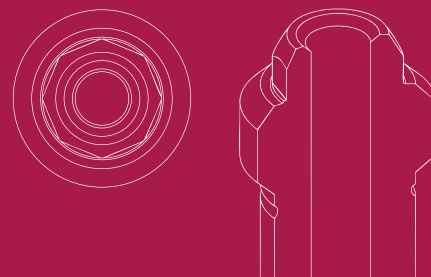

## LIST OF COMPATIBILITIES **AVAILABLE**

ANTHOGYR - DENTIUM - DENTIS - DIO IMPLANTS - EUROTEKNIKA - GT MEDICAL - IMPLANT DIRECT - MEGAGEN - PROCLINIC - STRAUMANN - TRINON - ZIMMER

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.323.074.01-2	31.313.074.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.110.01-2		
10	52.410.110.01-2	50.313.074.01-2	43.621.410.01-2 43.624.410.01-2
12	52.412.110.01-2		



LAB SCANBODY	SCANALOG
30.415.007.01-2	23.413.074.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.330.708.01-2	22.613.074.01-2	34.613.074.01-2
4	30°	33.430.708.01-2		
6		33.630.708.01-2		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.322.074.31-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		
CAPS		HEIGHT	TYPE	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.044.01-2	18	43.618.201.01-2
41.320.050.01-2	24	43.624.201.01-2
(IMPLANT DIRECT)	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.007.04-2	TORX T6	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm αs = Standard maximum angulation αc = Standard maximum angulation αd = Direct to implant maximum angulation

# COMPATIBLE WITH 0075

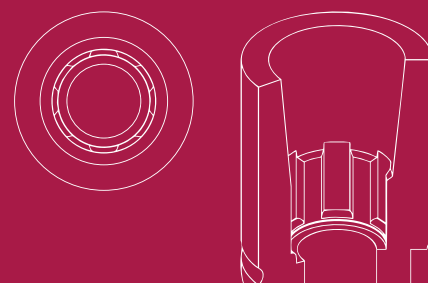

## LIST OF COMPATIBILITIES AVAILABLE

ANKLYOS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	42°	24°	31.322.075.01-2	-
2	20°	15°	31.322.075.02-2	31.312.075.02-2
3	20°	-	31.322.075.03-2	31.312.075.03-2
4	15°	-	31.322.075.04-2	31.312.075.04-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH-5mm	$\alpha_s$ CH-7mm	$\alpha_s$ CH-9mm	NON ENGAGING	ENGAGING
1	30°	20°	15°	31.322.075.21-2	-



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.105.01-2		43.621.410.01-2
12	52.412.105.01-2	50.312.075.03-2 (IG=3mm)	43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	ANALOG	DIGITAL ANALOG
3		33.330.734.01-2	22.612.075.01-2	34.612.075.01-2
4	25°	33.430.734.01-2		
6		33.630.734.01-2		



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE
54.315.075.21-2	49.414.000.01-2	6	A
	49.415.000.01-2	9	A
	49.416.000.01-2	13	A
	49.414.000.02-2	6	B
	49.415.000.02-2	9	B
	49.416.000.02-2	13	B
	49.414.000.03-2	6	C
	49.415.000.03-2	9	C
	49.416.000.03-2	13	C
	49.416.000.04-2	13	D
	49.416.000.05-2	13	E



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.318.077.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



## STRAIGHT SCREW

40.318.013.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	ENGAGING
2	42.302.075.02-2
3	42.302.075.03-2
4	42.302.075.04-2

[VIEW COMPONENTS](#)



### INTERNAL MULTI-UNIT


GH (mm)	ENGAGING
3	62.302.075.03-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO80

LIST OF COMPATIBILITIES **AVAILABLE**  
BIOHORIZONS - ZIMMER

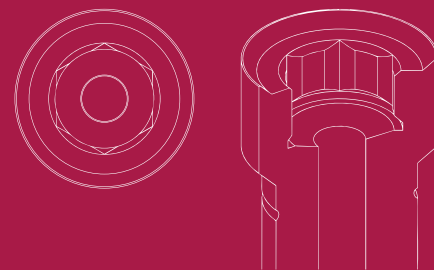


## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,4	45°	30°	31.324.080.01-2	31.314.080.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.124.01-2	50.314.080.01-2	43.621.410.01-2
12	52.412.124.01-2		43.624.410.01-2



### LAB SCANBODY

30.414.003.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3	30°	33.370.716.01-2
4		33.470.716.01-2
6		33.670.716.01-2

## ANALOG

ANALOG	DIGITAL ANALOG
22.614.080.01-2	34.614.080.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.080.21-2	49.414.000.01-2	6	A	43.601.104.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2		C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.317.071.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.317.004.01-2	Hex. 1.27	43.601.104.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm G1 = Standard maximum angulation G2 = Standard maximum angulation G3 = Direct to implant maximum angulation

# COMPATIBLE WITH OO81

## LIST OF COMPATIBILITIES AVAILABLE

BEGO

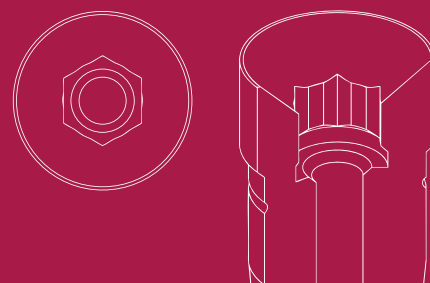

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,4	41°	18°	31.325.081.01-2	31.315.081.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.126.01-2	50.315.081.01-2	43.621.410.01-2
12	52.412.126.01-2		43.624.410.01-2



#### LAB SCANBODY

30.414.003.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.335.676.01-2	34.615.081.01 -2
4	30°	33.435.676.01-2	
6		33.635.676.01-2	

### ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.064.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.004.03-2	Hex. 1.25	43.601.104.01-2



# COMPATIBLE WITH OO82

LIST OF COMPATIBILITIES **AVAILABLE**  
KLOCKNER




## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	45°	25°	31.322.082.01-2	31.312.082.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.105.01-2	50.312.082.01-2	43.621.410.01-2
12	52.412.105.01-2		43.624.410.01-2



### LAB SCANBODY

30.412.001.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.345.804.01-2
4	25°	33.445.804.01-2
6		33.645.804.01-2

## ANALOG

DIGITAL ANALOG
34.612.082.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.074.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



### STRAIGHT SCREW

40.316.012.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT


GH (mm)	NON ENGAGING
1	42.302.082.01-2
2	42.302.082.02-2
3	42.302.082.03-2
4	42.302.082.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH 0083

LIST OF COMPATIBILITIES **AVAILABLE**  
KLOCKNER

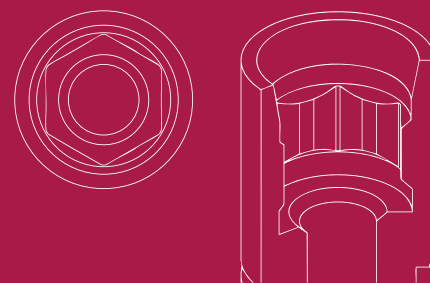


## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	45°	25°	31.323.083.01-2	31.313.083.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2		43.621.410.01-2
12	52.412.103.01-2	50.313.083.01-2	43.624.410.01-2



### LAB SCANBODY

30.413.002.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2	34.613.083.01-2
4	30°	33.445.856.01-2	
6		33.645.856.01-2	



## ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.076.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



### STRAIGHT SCREW

40.318.012.02-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.083.01-2
2	42.303.083.02-2
3	42.303.083.03-2
4	42.303.083.04-2


[VIEW COMPONENTS](#)



# COMPATIBLE WITH OO84

## LIST OF COMPATIBILITIES AVAILABLE

XIVE

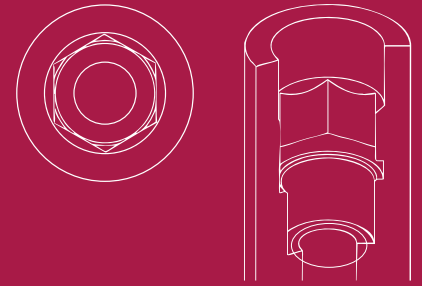

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	40°	-	31.321.084.01-2	31.311.084.01-2
<b>LAB SCANBODY</b>				
30.410.006.01-2				



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.314.076.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.003.03-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH OO85

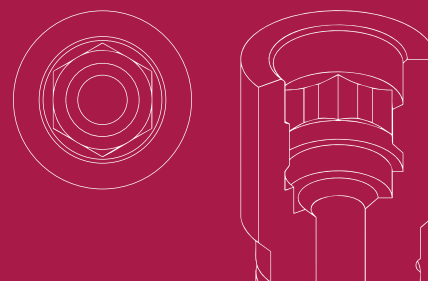

## LIST OF COMPATIBILITIES AVAILABLE XIVE

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,3	45°	30°	31.324.085.01-2	31.314.085.01-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_S$ CH=5mm	$\alpha_S$ CH=7mm	$\alpha_S$ CH=9mm	NON ENGAGING	ENGAGING
0,3	30°	25°	20°	-	31.314.085.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.117.01-2	50.314.085.01-2	43.621.410.01-2
12	52.412.117.01-2		43.624.410.01-2



#### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2	34.614.085.01-2
4	25°	33.445.856.01-2	
6		33.645.856.01-2	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.081.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.004.02-2	Hex. 1.25	43.601.104.01-2



# COMPATIBLE WITH OO86

LIST OF COMPATIBILITIES **AVAILABLE**  
XIVE

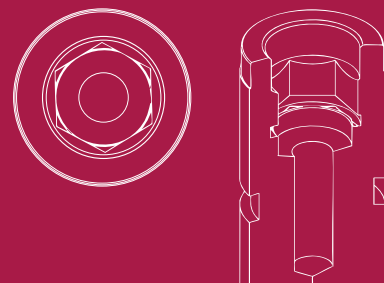


## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	45°	-	31.325.086.01-2	31.315.086.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.117.01-2		43.621.410.01-2
12	52.412.117.01-2	50.314.085.01-2	43.624.410.01-2



### LAB SCANBODY

30.415.007.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.345.856.01-2
4	25°	33.445.856.01-2
6		33.645.856.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.081.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.004.02-2	Hex. 1.25	43.601.104.01-2



# COMPATIBLE WITH OO87

## LIST OF COMPATIBILITIES AVAILABLE

CAMLOG



### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	25°	-	31.321.087.01-2	31.311.087.01-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,3	20°	20°	15°	-	31.311.087.21-2
2	25°	20°	15°	-	31.311.087.23-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.132.01-2		
12	52.412.132.01-2	50.311.087.04-2 (IG=3mm)	43.621.415.01-2



#### LAB SCANBODY

30.410.006.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.087.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.094.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.04-2	Hex. 1.27	43.625.105.01-2



# COMPATIBLE WITH OO88

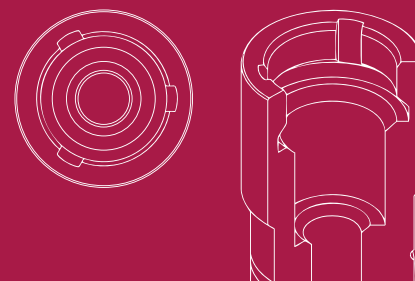

## LIST OF COMPATIBILITIES AVAILABLE CAMLOG

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	25°	-	31.324.088.01-2	31.314.088.01-2




#### LAB SCANBODY

30.414.003.01-2



### SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.088.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		

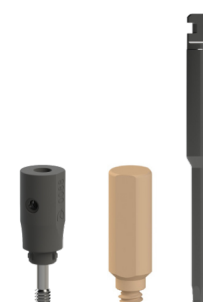

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.320.094.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.005.04-2	Hex. 1.27	43.625.105.01-2



# COMPATIBLE WITH 0090

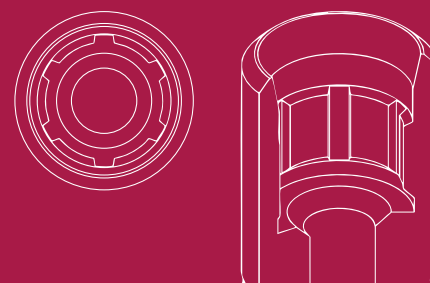

## LIST OF COMPATIBILITIES AVAILABLE

ASTRA

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	45°	24°	31.321.090.01-2	31.311.090.01-2
2	25°	-	31.321.090.02-2	31.311.090.02-2
3	20°	-	31.321.090.03-2	31.311.090.03-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH-5mm	$\alpha_s$ CH-7mm	$\alpha_s$ CH-9mm	NON ENGAGING	ENGAGING
1	30°	25°	15°	-	31.311.090.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.128.01-2	50.311.090.03-2 (IG=3mm)	43.621.415.01-2



#### LAB SCANBODY

30.410.006.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.325.472.01-2*	34.611.090.01-2
4	25°	33.425.472.01-2*	
6		33.625.472.01-2*	



\*Only for R  
\*Only for titanium and soft materials

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.090.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.314.074.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.005.01-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

# COMPATIBLE WITH 0091

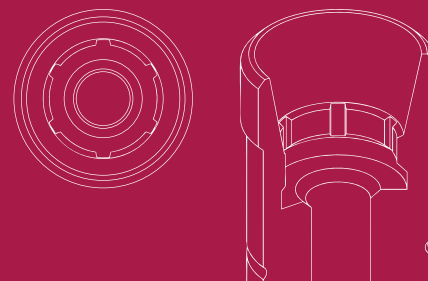

## LIST OF COMPATIBILITIES AVAILABLE

ASTRA

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	38°	18°	31.324.091.01-2	31.314.091.01-2
2	25°	-	31.324.091.02-2	31.314.091.02-2
3	20°	25°	31.324.091.03-2	31.314.091.03-2
4	15°	25°	31.324.091.04-2	31.314.091.04-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH-5mm	$\alpha_s$ CH-7mm	$\alpha_s$ CH-9mm	NON ENGAGING	ENGAGING
1,2	30°	25°	15°	-	31.314.091.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.102.01-2		43.621.410.01-2
12	52.412.102.01-2	50.314.091.03-2 (IG=3mm)	43.624.410.01-2



#### LAB SCANBODY

30.413.002.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.958.01-2	34.614.091.01-2
4	30°	33.490.958.01-2	
6		33.690.958.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.091.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.320.074.01-2	41.320.129.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.005.01-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT


GH (mm)	ENGAGING
1	42.303.091.01-2
2	42.303.091.02-2
3	42.303.091.03-2
4	42.303.091.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH 0092

LIST OF COMPATIBILITIES **AVAILABLE**  
ASTRA

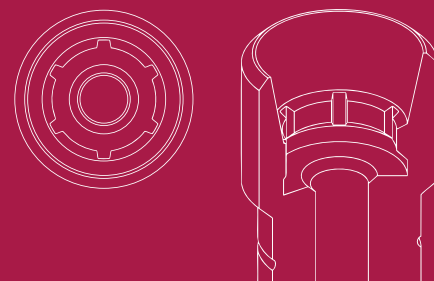

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	45°	25°	31.325.092.01-2	31.315.092.01-2
2	25°	-	31.325.092.02-2	31.315.092.02-2
3	20°	-	31.325.092.03-2	31.315.092.03-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1	30°	25°	15°	-	31.315.092.21-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.129.01-2	50.315.092.01-2 50.315.092.03-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2



### LAB SCANBODY

30.415.007.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.958.01-2	34.615.092.01-2
4	30°	33.490.958.01-2	
6		33.690.958.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.092.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.320.074.01-2	41.320.129.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.005.01-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_d$  = Standard maximum angulation  $\alpha_i$  = Direct to implant maximum angulation

# COMPATIBLE WITH 0096



## LIST OF COMPATIBILITIES **AVAILABLE**

ACE - ANTHOGRYR - DENTIUM - EUROTEKNIKA - IMPLANT DIRECT - PROCLINIC - SOUTHERN IMPLANTS - STRAUMANN

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.324.096.01-2	31.314.096.01-2



LAB SCANBODY	SCANALOG
30.414.008.01-2	23.414.096.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.315.708.01-2
4	30°	33.415.708.01-2
6		33.615.708.01-2

### ANALOG

ANALOG	DIGITAL ANALOG
22.614.096.01-2	34.614.096.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.096.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.067.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.007.01-2	TORX T6	43.601.107.01-2



# COMPATIBLE WITH O101

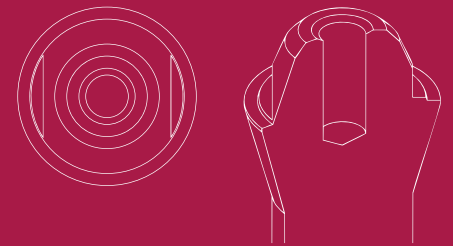

LIST OF COMPATIBILITIES **AVAILABLE**  
STRAUMANN

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	30°	31.323.101.01-2	-



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
9	52.409.133.01-2	50.313.101.01-2	43.621.410.01-2 43.624.410.01-2



LAB SCANBODY	MINI SCANBODY	SCANALOG
30.413.005.01-2	53.413.101.01-2	23.413.101.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.335.676.01-2	34.613.101.01-2
4	30°	33.435.676.01-2	
6		33.635.676.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

### SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.322.101.31-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		
	CAPS	HEIGHT	TYPE	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



### SCREWS


DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.314.043.01-2	41.314.050.31-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2
STRAIGHT SCREW	TYPE	SCREWDRIVER	
40.314.007.01-2	TORX T6	43.601.107.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH O102

LIST OF COMPATIBILITIES **AVAILABLE**  
BIOHORIZONS



## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,8	38°	18°	31.322.102.01-2	31.312.102.01-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1	30°	25°	20°	31.322.102.29-2	31.312.102.29-2
1,8	25°	15°	10°	31.322.102.21-2	31.312.102.21-2
3	20°	20°	15°	31.322.102.23-2	31.312.102.23-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.128.01-2	50.312.102.03-2 (IG=3mm)	43.621.415.01-2



LAB SCANBODY	SCANALOG
30.412.001.01-2	23.412.102.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

### DYNAMIC MILLING TOOL

### ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2	34.612.102.01-2
4	25°	33.445.856.01-2	
6		33.645.856.01-2	



### SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.102.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.317.065.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.317.005.02-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.102.01-2
2	42.302.102.02-2
3	42.302.102.03-2
4	42.302.102.04-2

[VIEW COMPONENTS](#)




### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
2,5/3,9	48.312.102.02-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH 0109



## LIST OF COMPATIBILITIES **AVAILABLE**

ASTRA - CORTEX - MOZO-GRAU (TICARE) - SOUTHERN IMPLANTS

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	45°	29°	31.322.109.01-2	31.312.109.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.128.01-2	50.312.109.01-2	43.621.415.01-2



#### LAB SCANBODY

30.412.001.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG	ANALOG
3		33.360.754.01-2*	34.612.109.01-2	22.612.109.01-2
4	25°	33.460.754.01-2*		
6		33.660.754.01-2*		

### ANALOG



\*Only for R

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.070.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.005.02-2	Hex. 1.27	43.625.105.01-2



# COMPATIBLE WITH O110

## LIST OF COMPATIBILITIES AVAILABLE

BRENT MEDICAL

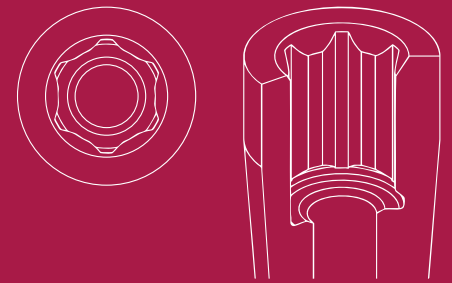


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,4	45°	30°	31.320.110.01-2	31.310.110.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.117.01-2		43.621.410.01-2
12	52.412.117.01-2	50.310.110.04-2 (IG=3mm)	43.624.410.01-2



#### LAB SCANBODY

30.410.006.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.756.01-2*	34.610.110.01-2
4	20°	33.460.756.01-2*	
6		33.660.756.01-2*	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.083.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.007.01-2	TORX T6	43.601.107.01-2



# COMPATIBLE WITH O111

## LIST OF COMPATIBILITIES AVAILABLE

BREIDENT MEDICAL

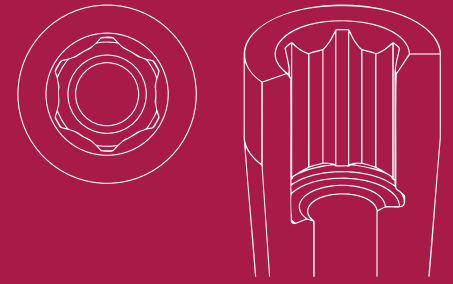


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,4	45°	30°	31.323.111.01-2	31.313.111.01-2
2,5	25°	-	-	31.313.111.03-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.117.01-2		43.621.410.01-2
12	52.412.117.01-2	50.310.110.04-2 (IG=3mm)	43.624.410.01-2



#### LAB SCANBODY

30.413.002.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.756.01-2	34.610.110.01-2
4	20°	33.460.756.01-2	
6		33.660.756.01-2	

### ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.083.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.003.06-2	TORX T6	43.601.107.01-2




## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.111.01-2
2	42.303.111.02-2
3	42.303.111.03-2
4	42.303.111.04-2

[VIEW COMPONENTS](#)



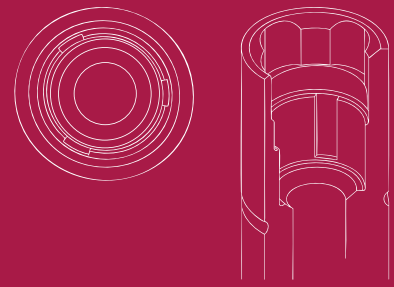

# COMPATIBLE WITH O119

## LIST OF COMPATIBILITIES AVAILABLE

BIOHORIZONS - CAMLOG


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	35°	-	31.321.119.01-2	31.311.119.01-2
2	30°	-	31.321.119.02-2	31.311.119.02-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.132.01-2		
12	52.412.132.01-2	50.311.119.03-2 (IG=3mm)	43.621.415.01-2



#### LAB SCANBODY

30.410.006.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.756.01-2	34.611.119.01-2
4	25°	33.460.756.01-2	
6		33.660.756.01-2	



### ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.119.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.080.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.07-2	Hex. 1.27	43.625.105.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.301.119.01-2
2	42.301.119.02-2
3	42.301.119.03-2
4	42.301.119.04-2

VIEW COMPONENTS



### ANGULATED MULTI-UNIT 20°


GH (mm)	ENGAGING
3.5/4.9	48.312.119.03-2

VIEW COMPONENTS



# COMPATIBLE WITH O120

LIST OF COMPATIBILITIES **AVAILABLE**  
BIOHORIZONS - CAMLOG

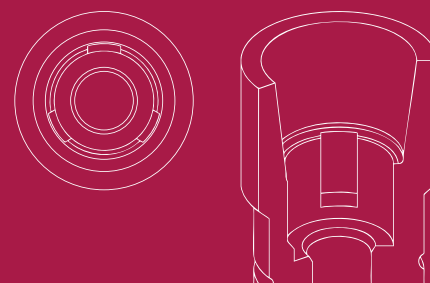

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	45°	25°	31.323.121.01-2	31.313.121.01-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
2	25°	20°	15°	-	31.313.121.22-2
3	25°	20°	10°	-	31.313.121.23-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.108.01-2		43.621.410.01-2
12	52.412.108.01-2	50.312.120.03-2 (IG=3mm)	43.624.410.01-2



### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

### DYNAMIC MILLING TOOL

### ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.754.01-2	34.612.120.01-2
4	20°	33.460.754.01-2	
6		33.660.754.01-2	



### SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.121.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.080.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.07-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.121.01-2
2	42.303.121.02-2
3	42.303.121.03-2
4	42.303.121.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
2,5/3,9	48.312.120.02-2
3,5/4,9	48.312.120.03-2

[VIEW COMPONENTS](#)



### INTERNAL MULTI-UNIT


GH (mm)	ENGAGING
2	62.303.121.02-2
4	62.303.121.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH O121

LIST OF COMPATIBILITIES **AVAILABLE**  
CAMLOG



## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	45°	25°	31.323.121.01-2	31.313.121.01-2




## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
2	25°	20°	15°	-	31.313.121.22-2
3	25°	20°	10°	-	31.313.121.23-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.109.01-2	50.313.121.01-2	43.621.410.01-2
12	52.412.109.01-2	50.313.121.03-2 (IG=3mm)	43.624.410.01-2



### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.754.01-2	34.613.121.01-2
4	20°	33.460.754.01-2	
6		33.660.754.01-2	



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.121.21-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.080.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.07-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.121.01-2
2	42.303.121.02-2
3	42.303.121.03-2
4	42.303.121.04-2

[VIEW COMPONENTS](#)




### INTERNAL MULTI-UNIT

GH (mm)	ENGAGING
2	62.303.121.02-2
4	62.303.121.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH O124

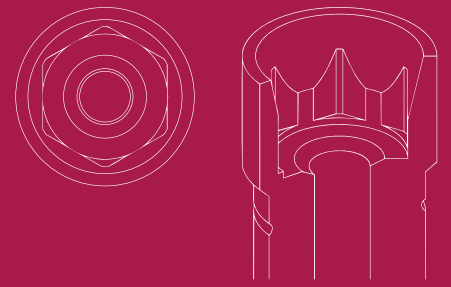

## LIST OF COMPATIBILITIES **AVAILABLE**

HAHN IMPLANT (GLIDEWELL) - NOBEL BIOCARE

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,4	42°	19°	31.324.124.01-2	31.314.124.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.125.01-2	50.314.124.01-2	43.621.410.01-2 43.624.410.01-2



#### LAB SCANBODY

30.414.003.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.335.758.01-2	34.614.124.01-2
4	30°	33.435.758.01-2	
6		33.635.758.01-2	

### ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.124.21-2	49.414.000.01-2	6	A	43.625.108.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.075.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.008.02-2	UNIGRIP	43.625.108.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH O125

LIST OF COMPATIBILITIES **AVAILABLE**  
MEDENTIS



## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,1	42°	20°	31.323.125.01-2	31.313.125.01-2
2	25°	15°	31.323.125.02-2	31.313.125.02-2




## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,1	30°	25°	15°	31.323.125.21-2	31.313.125.21-2
3	20°	15°	10°	-	31.313.125.23-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.117.01-2	50.313.125.01-2	43.621.410.01-2
12	52.412.117.01-2		43.624.410.01-2



### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**DYNAMIC MILLING TOOL**

**ANALOG**

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.315.804.01-2	34.613.125.01-2
4	25°	33.415.804.01-2	
6		33.615.804.01-2	



**SCANBODY OP**

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.125.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



**SCREWS**

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
41.316.078.01-2	41.316.124.01-2	18	43.618.201.01-2
		24	43.624.201.01-2
		32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.01-2	TORX T6	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.125.01-2
2	42.303.125.02-2
3	42.303.125.03-2
4	42.303.125.04-2

VIEW COMPONENTS



### ANGULATED MULTI-UNIT 20°


GH (mm)	ENGAGING
1,5/2,9	48.312.125.01-2
2,5/3,9	48.312.125.02-2
3,5/4,9	48.312.125.03-2

VIEW COMPONENTS



# COMPATIBLE WITH O128

LIST OF COMPATIBILITIES **AVAILABLE**  
MEGAGEN

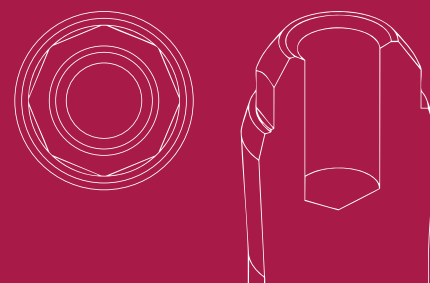

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
2,5	45°	30°	31.322.128.01-2	-
<b>LAB SCANBODY</b>				
30.413.002.01-2				



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.044.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.003.05-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

# COMPATIBLE WITH O129

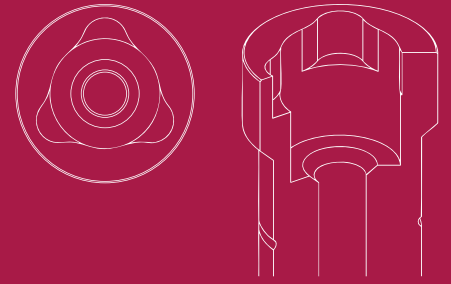

## LIST OF COMPATIBILITIES **AVAILABLE**

NOBEL BIOCARE - SOUTHERN IMPLANTS


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	35°	30°	31.325.129.01-2	31.315.129.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.130.01-2	50.315.129.01-2	43.621.410.01-2 43.624.410.01-2



#### LAB SCANBODY

30.415.007.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG	ANALOG
3		33.390.958.01-2	34.615.129.01-2	22.615.129.01-2
4	30°	33.490.958.01-2		
6		33.690.958.01-2		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.320.090.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.008.03-2	UNIGRIP	43.625.108.01-2



# COMPATIBLE WITH O130

## LIST OF COMPATIBILITIES AVAILABLE

DENTAURUM

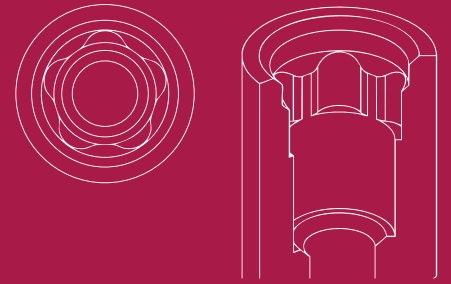

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,5	30°	29°	31.322.130.01-2	31.312.130.01-2
<b>LAB SCANBODY</b>				
30.412.001.01-2				



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.081.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.08-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

# COMPATIBLE WITH O131

LIST OF COMPATIBILITIES **AVAILABLE**  
DENTAURUM

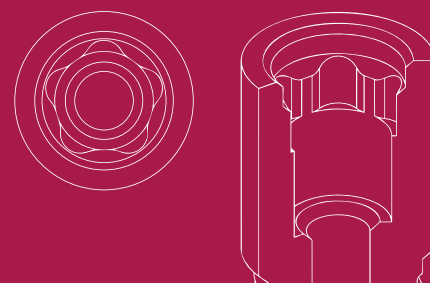

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	29°	31.323.131.01-2	31.313.131.01-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,5	30°	20°	15°	31.323.131.21-2	31.313.131.21-2



## LAB SCANBODY

30.413.002.01-2



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.081.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.08-2	Hex. 1.27	43.625.105.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O132

LIST OF COMPATIBILITIES **AVAILABLE**  
DENTAURUM

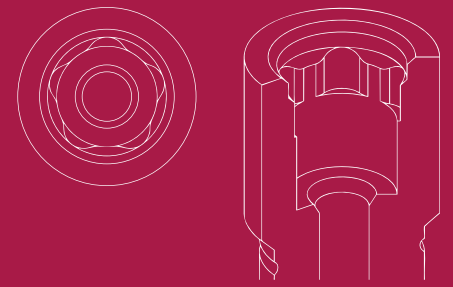

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	28°	31.324.132.01-2	31.314.132.01-2



### LAB SCANBODY

30.414.003.01-2



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.081.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.005.08-2	Hex. 1.27	43.625.105.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O135

LIST OF COMPATIBILITIES **AVAILABLE**

STRAUMANN

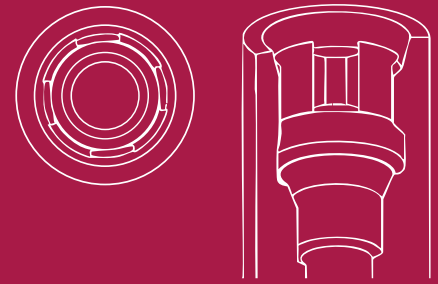

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	45°	30°	31.320.135.01-2	31.310.135.01-2



### LAB SCANBODY

30.410.006.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.315.804.01-2
4	25°	33.415.804.01-2
6		33.615.804.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.135.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.314.080.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.007.02-2	TORX T6	43.601.107.01-2



# COMPATIBLE WITH O136

## LIST OF COMPATIBILITIES AVAILABLE

ALPHABIO

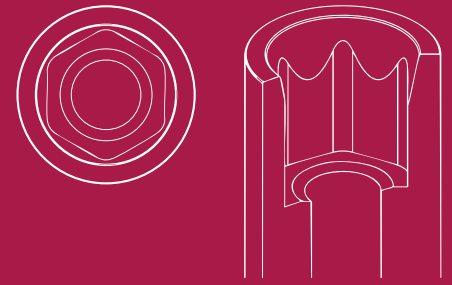

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,7	45°	30°	31.320.136.01-2	31.310.136.01-2
1,5	25°	20°	31.320.136.02-2	31.310.136.02-2
3	20°	-	31.320.136.04-2	31.310.136.04-2
4	20°	-	31.320.136.05-2	31.310.136.05-2
5	15°	-	31.320.136.06-2	31.310.136.06-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.128.01-2	50.310.136.01-2 50.310.136.04-2 (IG=3mm)	43.621.415.01-2



#### LAB SCANBODY

30.410.006.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.754.01-2	34.610.136.01-2
4	25°	33.460.754.01-2	
6		33.660.754.01-2	

### ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.071.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.004.03-2	Hex. 1.25	43.601.104.01-2



## MULTI-UNIT


### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.300.136.01-2
2	42.300.136.02-2
3	42.300.136.03-2
4	42.300.136.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH O137

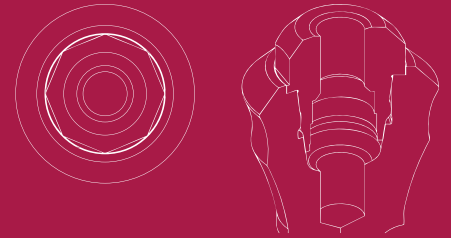

## LIST OF COMPATIBILITIES AVAILABLE

STRAUMANN

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,6	45°	30°	31.324.137.01-2	31.314.137.01-2



#### LAB SCANBODY

30.414.008.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.044.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.320.007.04-2	TORX T6	43.601.107.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

# COMPATIBLE WITH O145

## LIST OF COMPATIBILITIES AVAILABLE

ADIN

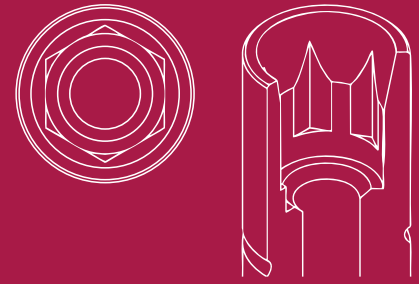

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	45°	-	31.320.145.01-2	31.310.145.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY
10	52.410.128.01-2



LAB SCANBODY
30.410.006.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.315.078.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.005.01-2	Hex. 1.27	43.601.105.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O149

## LIST OF COMPATIBILITIES AVAILABLE

ANTHOGYR

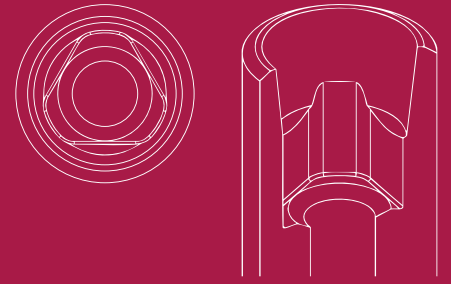


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	45°	29°	31.323.149.01-2	31.313.149.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.132.01-2	50.310.161.01-2	43.621.415.01-2
12	52.412.132.01-2		



#### LAB SCANBODY

30.413.002.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.320.704.01-2*	34.610.161.01-2
4	25°	33.420.704.01-2*	
6		33.620.704.01-2*	

\*Only for R



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.079.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



### STRAIGHT SCREW

40.316.014.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.161.01-2
2	42.302.161.02-2
3	42.302.161.03-2

[VIEW COMPONENTS](#)




### ANGULATED MULTI-UNIT 20°

GH (mm)	NON ENGAGING
3/4,4	48.312.161.05-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH O150

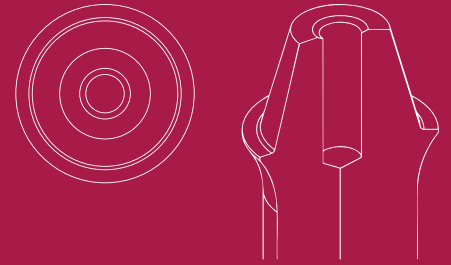

## LIST OF COMPATIBILITIES AVAILABLE

BEGO

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,5	45°	-	31.323.150.01-2	-
<b>LAB SCANBODY</b>				
30.413.005.01-2				



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.046.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

# COMPATIBLE WITH O151

## LIST OF COMPATIBILITIES AVAILABLE

BTI

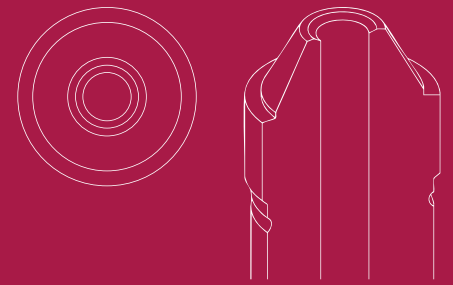

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	30°	31.323.151.01-2	-



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
9	52.409.123.01-2	50.313.151.01-2	43.621.410.01-2 43.624.410.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.613.151.01-2
4	30°	33.490.716.01-2	
6		33.690.716.01-2	

### ANALOG



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.039.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.008.01-2	UNIGRIP	43.625.108.01-2



# COMPATIBLE WITH O158

LIST OF COMPATIBILITIES **AVAILABLE**  
IMPLANT DIRECT

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER	
54.322.158.31-2	49.414.000.01-2	6	A	43.625.105.01-2	
	49.415.000.01-2	9	A		
	49.416.000.01-2	13	A		
	49.414.000.02-2	6	B		
	49.415.000.02-2	9	B		
	49.416.000.02-2	13	B		
	49.414.000.03-2	6	C		
	49.415.000.03-2	9	C		
	49.416.000.03-2	13	C		
	49.416.000.04-2	13	D		
	49.416.000.05-2	13	E		
		CAPS	HEIGHT		TYPE
		49.418.000.01-2	3,8		Regular
		49.418.000.02-2	3,8		Wide
		49.419.000.01-2	6		Regular
	49.419.000.02-2	6	Wide		
	49.420.000.01-2	8	Regular		
	49.420.000.02-2	8	Wide		




## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.317.040.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH O159

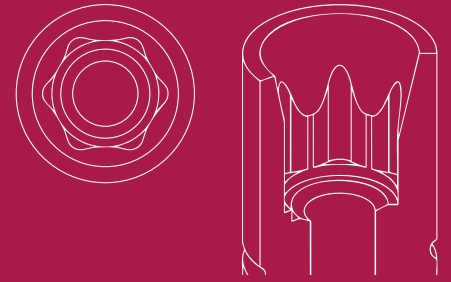

## LIST OF COMPATIBILITIES **AVAILABLE**

HAHN IMPLANT (GLIDEWELL) - NOBEL BIOCARE - REFLECT


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	41°	17°	31.320.159.01-2	31.310.159.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.128.01-2	50.310.159.01-2	43.621.415.01-2



#### LAB SCANBODY

30.410.006.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG	ANALOG
3		33.335.754.01-2*	34.610.159.01-2	22.610.159.01-2
4	25°	33.435.754.01-2*		
6		33.635.754.01-2*		



\*Only for R

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.067.02-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.008.02-2	UNIGRIP	43.625.108.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.300.159.01-2
2	42.300.159.02-2
3	42.300.159.03-2
4	42.300.159.04-2


[VIEW COMPONENTS](#)



# COMPATIBLE WITH O160

## LIST OF COMPATIBILITIES AVAILABLE

STRAUMANN

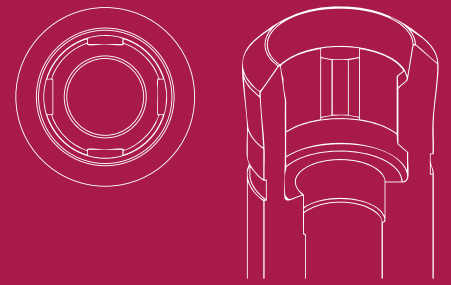


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	30°	31.320.160.01-2	31.310.160.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.131.01-2	50.310.160.01-2	43.621.415.01-2



LAB SCANBODY	SCANALOG
30.410.006.01-2	23.410.160.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG	ANALOG
3		33.315.804.01-2	34.610.160.01-2	22.610.160.01-2
4	25°	33.415.804.01-2		
6		33.615.804.01-2		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.078.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.01-2	TORX T6	43.601.107.01-2



# COMPATIBLE WITH O161

## LIST OF COMPATIBILITIES AVAILABLE

ANTHOGYR

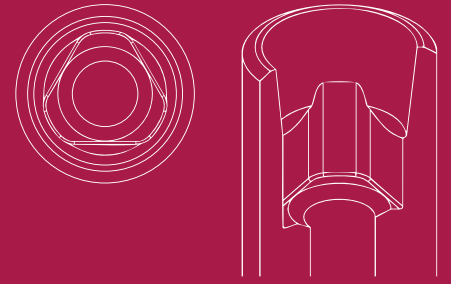

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	45°	25°	31.320.161.01-2	31.310.161.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.132.01-2	50.310.161.01-2	43.621.415.01-2
12	52.412.132.01-2		



#### LAB SCANBODY

30.410.006.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.320.704.01-2*	34.610.161.01-2
4	25°	33.420.704.01-2*	
6		33.620.704.01-2*	

\*Only for R



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.079.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



### STRAIGHT SCREW

40.316.014.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.161.01-2
2	42.302.161.02-2
3	42.302.161.03-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	NON ENGAGING
3/4,4	48.312.161.05-2


[VIEW COMPONENTS](#)



# COMPATIBLE WITH O162

## LIST OF COMPATIBILITIES AVAILABLE

ANTHOGYR

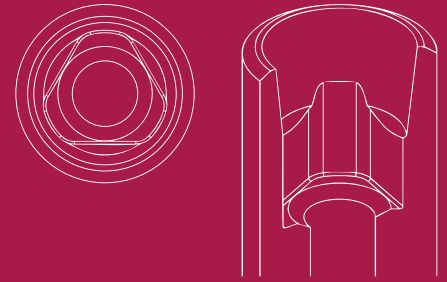


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	45°	24°	31.324.162.01-2	31.314.162.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.132.01-2	50.310.161.01-2	43.621.415.01-2
12	52.412.132.01-2		



#### LAB SCANBODY

30.414.003.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.320.704.01-2*	34.610.161.01-2
4	25°	33.420.704.01-2*	
6		33.620.704.01-2*	

\*Only for R



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.079.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




## STRAIGHT SCREW

40.316.014.01-2



# COMPATIBLE WITH O163

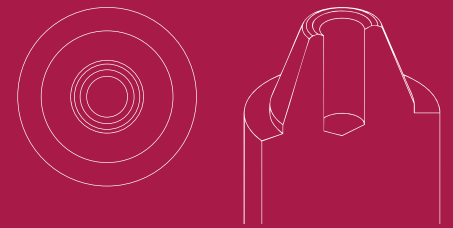

## LIST OF COMPATIBILITIES AVAILABLE

ANTHOGYR

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	30°	31.323.163.01-2	-



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.112.01-2	50.313.163.01-2	43.620.411.01-2



#### LAB SCANBODY

30.413.005.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.613.163.01-2
4	30°	33.490.716.01-2	
6		33.690.716.01-2	

### ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.039.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



## STRAIGHT SCREW


40.314.014.01-2



# COMPATIBLE WITH O166

## LIST OF COMPATIBILITIES AVAILABLE

LASAK

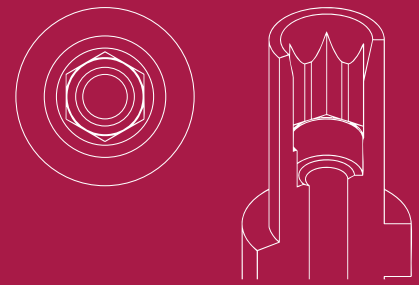

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,9	45°	30°	31.320.166.01-2	31.310.166.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.128.01-2	50.310.166.03-2 (IG=3mm)	43.621.415.01-2



#### LAB SCANBODY

30.410.006.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.335.754.01-2	34.610.166.01-2
4	25°	33.435.754.01-2	
6		33.635.754.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation


**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.084.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH O167

LIST OF COMPATIBILITIES **AVAILABLE**  
LASAK

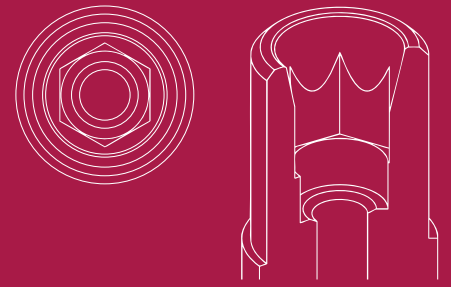

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,9	43°	30°	31.322.167.01-2	31.312.167.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.117.01-2	50.313.167.03-2 (IG=3mm)	43.621.410.01-2
12	52.412.117.01-2		43.624.410.01-2



### LAB SCANBODY

30.412.001.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.330.734.01-2	34.613.167.01-2
4	20°	33.430.734.01-2	
6		33.630.734.01-2	

## ANALOG




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation


**SCREWS**

DYNAMIC SCREW	LENTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.084.02-2	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.004.01-2	Hex. 1.25	43.601.104.01-2

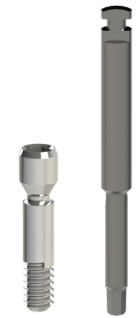

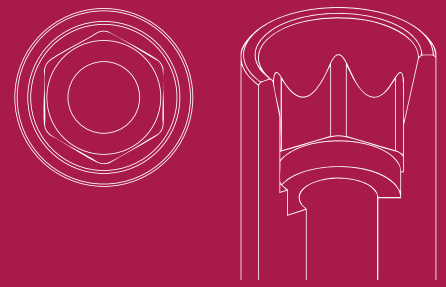

# COMPATIBLE WITH O169

## LIST OF COMPATIBILITIES AVAILABLE

ALPHABIO

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,6	45°	29°	31.322.169.01-2	31.312.169.01-2
1,5	25°	15°	31.322.169.02-2	31.312.169.02-2
3	20°	-	31.322.169.04-2	31.312.169.04-2




### DYNAMIC 3TIBASE

GH (mm)	$\alpha_S$ CH=5mm	$\alpha_S$ CH=7mm	$\alpha_S$ CH=9mm	NON ENGAGING	ENGAGING
1,5	30°	25°	15°	31.322.169.22-2	31.312.169.22-2
3	25°	20°	15°	31.322.169.24-2	31.312.169.24-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.117.01-2	50.312.169.01-2	43.621.410.01-2
12	52.412.117.01-2	50.312.169.04-2 (IG=3mm)	43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.330.734.01-2	34.612.169.01-2
4	25°	33.430.734.01-2	
6		33.630.734.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.169.21-2	49.414.000.01-2	6	A	43.601.104.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.317.070.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.169.01-2
2	42.302.169.02-2
3	42.302.169.03-2
4	42.302.169.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
1,5/2,9	48.312.169.01-2
2,5/3,9	48.312.169.02-2
3,5/4,9	48.312.169.03-2

[VIEW COMPONENTS](#)




### INTERNAL MULTI-UNIT

GH (mm)	ENGAGING
3	62.302.169.03-2
4	62.302.169.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH O170

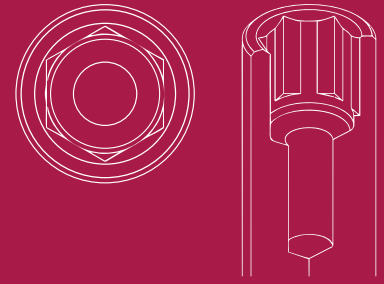

## LIST OF COMPATIBILITIES AVAILABLE

SIC INVENT

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
0,3	38°	-	31.322.170.01-2	31.312.170.01-2



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_S$ CH=5mm	$\alpha_S$ CH=7mm	$\alpha_S$ CH=9mm	NON ENGAGING	ENGAGING
0,3	30°	20°	15°	31.322.170.21-2	31.312.170.21-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY
10	52.410.104.01-2
12	52.412.104.01-2



LAB SCANBODY
30.410.006.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.390.716.01-2
4	25°	33.490.716.01-2
6		33.690.716.01-2



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.170.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.079.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH O171

## LIST OF COMPATIBILITIES AVAILABLE

SIC INVENT

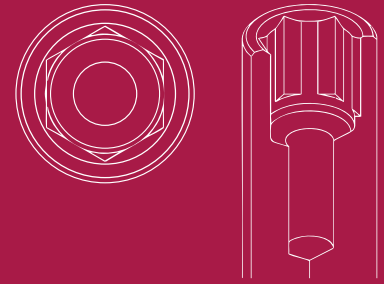

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	35°	-	31.323.171.01-2	31.313.171.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY
10	52.410.117.01-2
12	52.412.117.01-2



LAB SCANBODY
30.412.001.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.390.716.01-2
4	25°	33.490.716.01-2
6		33.690.716.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.170.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	




## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.079.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH O173

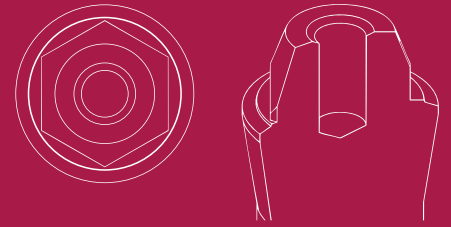

## LIST OF COMPATIBILITIES AVAILABLE

KLOCKNER

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	30°	31.323.173.01-2	-
<b>LAB SCANBODY</b>				
30.413.005.01-2				



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.040.02-2	24	43.624.201.01-2
	32	43.632.201.01-2




### STRAIGHT SCREW

40.314.012.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

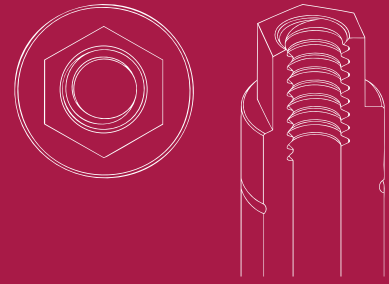

# COMPATIBLE WITH O176

LIST OF COMPATIBILITIES **AVAILABLE**  
EASY IMPLANT

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	35°	-	-	31.310.176.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.138.01-2	50.310.176.01-2	43.621.415.01-2



### LAB SCANBODY

30.410.006.01-2



## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.756.01-2	34.610.176.01-2
4	35°	33.460.756.01-2	
6		33.660.756.01-2	




## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.044.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

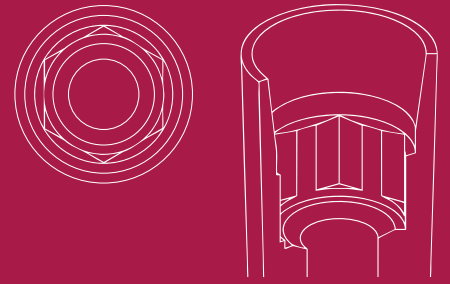

# COMPATIBLE WITH O178

## LIST OF COMPATIBILITIES AVAILABLE

P-I BRANEMARK - ZIMMER

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
1,5	45°	-	31.320.178.01-2	31.310.178.01-2



#### LAB SCANBODY

30.410.006.01-2



### ANALOG

#### DIGITAL ANALOG

34.610.178.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.080.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



### MULTI-UNIT

#### INTERNAL MULTI-UNIT


GH (mm)	NON ENGAGING
3	62.300.178.03-2
4	62.300.178.04-2

[VIEW COMPONENTS](#)



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

# COMPATIBLE WITH O181

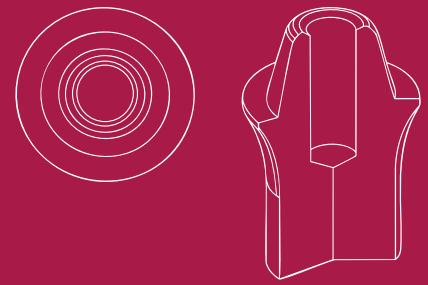

## LIST OF COMPATIBILITIES AVAILABLE

PALTOP - SURCAM DENTAL

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,4	45°	-	31.322.181.01-2	-



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,4	30°	30°	20°	31.322.181.21-2	-



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.112.01-2	50.312.181.01-2	43.620.411.01-2



LAB SCANBODY	SCANALOG
30.413.005.01-2	23.412.181.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.360.756.01-2	34.612.181.01-2
4	30°	33.460.756.01-2	
6		33.660.756.01-2	

### ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.322.181.31-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	
	CAPS	HEIGHT	TYPE	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
49.419.000.02-2	6	Wide		
49.420.000.01-2	8	Regular		
49.420.000.02-2	8	Wide		



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.318.043.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH O183

LIST OF COMPATIBILITIES **AVAILABLE**  
ANKLYOS

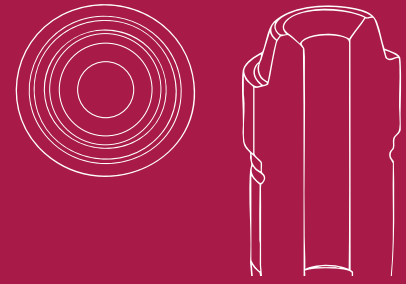


## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	-	31.322.183.01-2	-



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.136.01-2	50.312.183.01-2	43.620.411.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.330.734.01-2	34.612.183.01-2
4	30°	33.430.734.01-2	
6		33.630.734.01-2	

## ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE
54.322.183.31-2	49.414.000.01-2	6	A
	49.415.000.01-2	9	A
	49.416.000.01-2	13	A
	49.414.000.02-2	6	B
	49.415.000.02-2	9	B
	49.416.000.02-2	13	B
	49.414.000.03-2	6	C
	49.415.000.03-2	9	C
	49.416.000.03-2	13	C
	49.416.000.04-2	13	D
	49.416.000.05-2	13	E
	CAPS	HEIGHT	TYPE
	49.418.000.01-2	3,8	Regular
	49.418.000.02-2	3,8	Wide
	49.419.000.01-2	6	Regular
49.419.000.02-2	6	Wide	
49.420.000.01-2	8	Regular	
49.420.000.02-2	8	Wide	




## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.048.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH O186

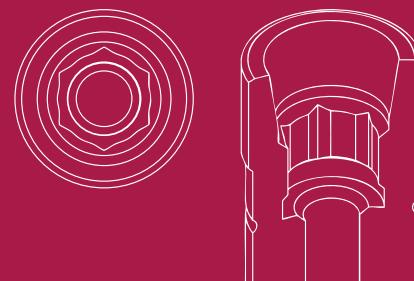

LIST OF COMPATIBILITIES **AVAILABLE**  
NEODENT

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	40°	30°	31.323.186.01-2	31.313.186.01-2
2,5	20°	18°	31.323.186.02-2	31.313.186.02-2
3,5	15°	-	31.323.186.03-2	31.313.186.03-2




## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,2	30°	25°	15°	31.323.186.21-2	31.313.186.21-2
2,5	30°	25°	15°	31.323.186.22-2	31.313.186.22-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.101.01-2		
10	52.410.101.01-2	50.313.186.04-2 (IG=3mm)	43.621.410.01-2 43.624.410.01-2
12	52.412.101.01-2		



### LAB SCANBODY

30.413.002.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.330.734.01-2	34.613.186.01-2
4	25°	33.430.734.01-2	
6		33.630.734.01-2	



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE
54.315.186.21-2	49.414.000.01-2	6	A
	49.415.000.01-2	9	A
	49.416.000.01-2	13	A
	49.414.000.02-2	6	B
	49.415.000.02-2	9	B
	49.416.000.02-2	13	B
	49.414.000.03-2	6	C
	49.415.000.03-2	9	C
	49.416.000.03-2	13	C
	49.416.000.04-2	13	D
49.416.000.05-2	13	E	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.084.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2
STRAIGHT SCREW		
40.316.008.04-2		



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.303.186.01-2
2	42.303.186.02-2
3	42.303.186.03-2
4	42.303.186.04-2
5	42.303.186.05-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
1,5/2,9	48.312.186.01-2
2,5/3,9	48.312.186.02-2
3,5/4,9	48.312.186.03-2

[VIEW COMPONENTS](#)



### INTERNAL MULTI-UNIT

GH (mm)	NON ENGAGING
2	62.303.186.02-2
3	62.303.186.03-2
4	62.303.186.04-2


[VIEW COMPONENTS](#)



# COMPATIBLE WITH O187

## LIST OF COMPATIBILITIES AVAILABLE

BEGO

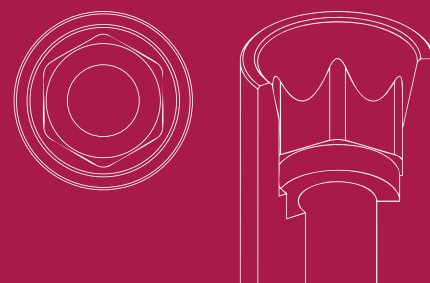


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	25°	31.322.009.01-2	31.312.009.01-2
0,5	25°	25°	31.322.009.02-2	31.312.009.02-2
1	25°	-	31.322.009.03-2	31.312.009.03-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.114.01-2	50.312.187.01-2	43.621.410.01-2
12	52.412.114.01-2		43.624.410.01-2



#### LAB SCANBODY

30.412.001.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.390.716.01-2	34.612.187.01-2
4	25°	33.490.716.01-2	
6		33.690.716.01-2	



### ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.059.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH O188

## LIST OF COMPATIBILITIES AVAILABLE

ADIN

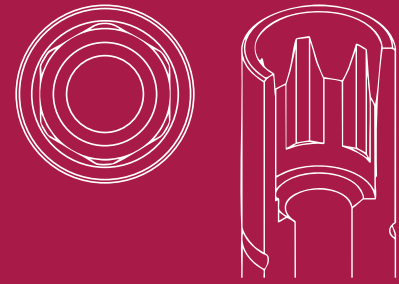

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	45°	-	31.320.188.01-2	31.310.188.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY
10	52.410.128.01-2



LAB SCANBODY
30.410.006.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.315.078.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O190



## LIST OF COMPATIBILITIES AVAILABLE DENTIUM

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,8	45°	-	31.320.190.01-2	31.310.190.01-2



#### LAB SCANBODY

30.410.006.01-2



### SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.084.02-2	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O191

LIST OF COMPATIBILITIES **AVAILABLE**  
DENTIUM

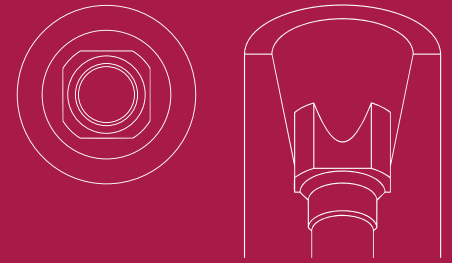

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,8	45°	-	31.322.191.01-2	31.312.191.01-2



### LAB SCANBODY

30.412.001.01-2



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.084.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.003.01-2	Hex. 1.20	43.601.103.02-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O192

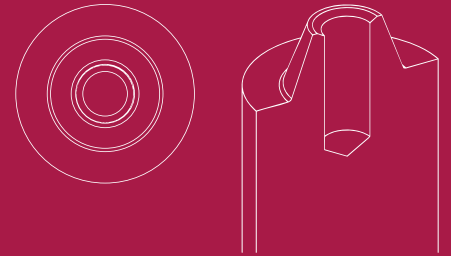

LIST OF COMPATIBILITIES **AVAILABLE**  
DENTIUM

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	-	31.323.192.01-2	-



LAB  
SCANBODY

30.413.005.01-2




## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.048.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O193

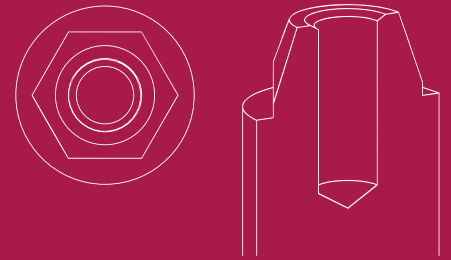

## LIST OF COMPATIBILITIES AVAILABLE

COWELLMEDI - DENTIUM

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	-	31.323.193.01-2	-
<b>LAB SCANBODY</b>				
30.413.005.01-2				



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.345.856.01-2
4	0°	33.445.856.01-2
6		33.645.856.01-2

### ANALOG

DIGITAL ANALOG
34.613.193.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.322.193.31-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	
CAPS		HEIGHT	TYPE	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.318.051.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.005.01-2	-	43.601.105.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm αs = Standard maximum angulation αc = Standard maximum angulation αd = Direct to implant maximum angulation

# COMPATIBLE WITH O195

## LIST OF COMPATIBILITIES AVAILABLE

ALPHABIO

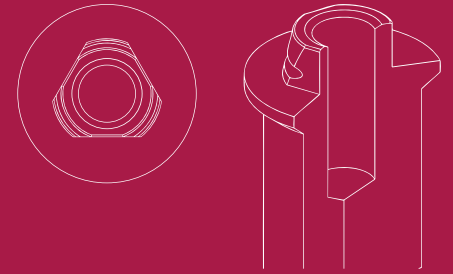

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	-	31.323.195.01-2	-



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,5	30°	25°	25°	31.323.195.21-2	-



### LAB SCANBODY

30.413.005.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.390.716.01-2
4	25°	33.490.716.01-2
6		33.690.716.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
54.322.195.31-2	49.416.000.04-2	13	D	43.601.104.01-2
	49.416.000.05-2	13	E	



CAPS	HEIGHT	TYPE
49.418.000.01-2	3,8	Regular
49.418.000.02-2	3,8	Wide
49.419.000.01-2	6	Regular
49.419.000.02-2	6	Wide
49.420.000.01-2	8	Regular
49.420.000.02-2	8	Wide

## SCREWS

DYNAMIC SCREW	HIGH	LENGTH	SCREWDRIVER
		18	43.618.201.01-2
41.317.041.01-2	41.317.052.36-2	24	43.624.201.01-2
		32	43.632.201.01-2




LIBRARY OPTIONS: GH - Gingival Height CH - Cement Height H - Height IG - Adaptor 3mm Gs - Standard maximum angulation Gc - Standard maximum angulation Gd - Direct to implant maximum angulation

# COMPATIBLE WITH O196

## LIST OF COMPATIBILITIES AVAILABLE

GC TECH

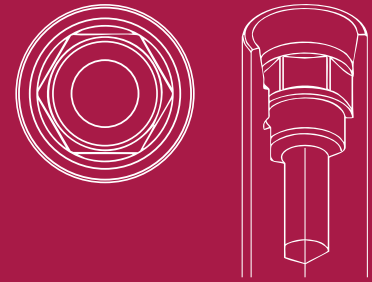

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	40°	-	31.320.196.01-2	31.310.196.01-2
2	25°	-	31.320.196.02-2	31.310.196.02-2
3	25°	-	31.320.196.03-2	31.310.196.03-2



#### LAB SCANBODY

30.410.006.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.086.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O197

## LIST OF COMPATIBILITIES AVAILABLE

GC TECH

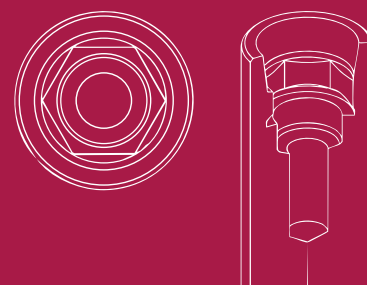

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,2	35°	25°	31.322.197.01-2	31.312.197.01-2
2	20°	25°	31.322.197.02-2	31.312.197.02-2
3	20°	-	31.322.197.03-2	31.312.197.03-2



### LAB SCANBODY

30.412.001.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.086.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O198

## LIST OF COMPATIBILITIES AVAILABLE

GC TECH

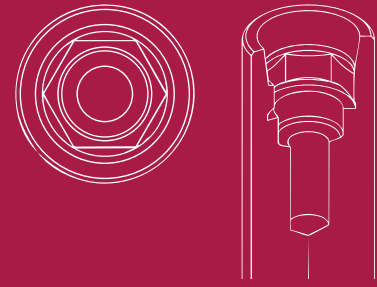

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_S$	$\alpha_C$	NON ENGAGING	ENGAGING
1,2	40°	-	31.324.198.01-2	31.314.198.01-2



#### LAB SCANBODY

30.414.003.01-2




### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.086.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_S$  = Standard maximum angulation  $\alpha_C$  = Standard maximum angulation  $\alpha_D$  = Direct to implant maximum angulation

# COMPATIBLE WITH O205

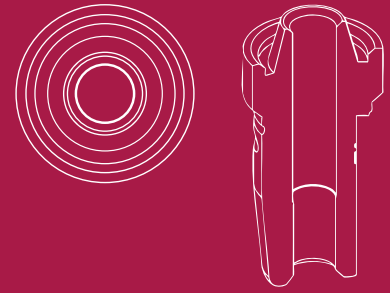

## LIST OF COMPATIBILITIES AVAILABLE

ZIMMER


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	-	31.322.205.01-2	-



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.112.01-2	50.312.205.01-2	43.620.411.01-2



#### LAB SCANBODY

30.412.001.01-2




### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.390.716.01-2
4	30°	33.490.716.01-2
6		33.690.716.01-2

### ANALOG

DIGITAL ANALOG
34.612.205.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.322.205.31-2	49.414.000.01-2	6	A	43.625.105.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	
		CAPS	HEIGHT	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



## SCREWS



DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.317.040.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm αs = Standard maximum angulation αc = Standard maximum angulation αd = Direct to implant maximum angulation

# COMPATIBLE WITH O207

LIST OF COMPATIBILITIES **AVAILABLE**  
STRAUMANN



## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	35°	15°	31.320.207.01-2	31.310.207.01-2
3	20°	-	31.320.207.03-2	31.310.207.03-2
4	15°	-	31.320.207.04-2	31.310.207.04-2



## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
1,5	25°	20°	15°	31.320.207.21-2	31.310.207.21-2
3	20°	15°	10°	31.320.207.23-2	31.310.207.23-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.310.207.03-2 (IG=3mm)	43.621.410.01-2
12	52.412.103.01-2		43.624.410.01-2



### LAB SCANBODY

30.410.006.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2*	34.610.207.01-2
4	30°	33.445.856.01-2*	
6		33.645.856.01-2*	



\*Only for R

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.207.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.066.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.03-2	TORX T6	43.601.107.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.207.01-2
2	42.302.207.02-2
3	42.302.207.03-2
4	42.302.207.04-2

[VIEW COMPONENTS](#)




### ANGULATED MULTI-UNIT 20°

GH (mm)	ENGAGING
2.5/3.9	48.312.207.02-2
3.5/4.9	48.312.207.03-2
4.5/5.9	48.312.207.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH O2O8

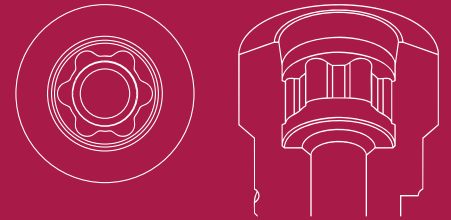

## LIST OF COMPATIBILITIES AVAILABLE

STRAUMANN


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	45°	20°	31.324.208.01-2	31.314.208.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.310.207.03-2 (IG=3mm)	43.621.410.01-2
12	52.412.103.01-2		43.624.410.01-2



#### LAB SCANBODY

30.414.003.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2*	34.614.208.01-2
4	30°	33.445.856.01-2*	
6		33.645.856.01-2*	

\*Only for R



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.207.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
	49.416.000.05-2	13	E	



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.066.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.03-2	TORX T6	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm G1 = Standard maximum angulation G2 = Standard maximum angulation G3 = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.207.01-2
2	42.302.207.02-2
3	42.302.207.03-2
4	42.302.207.04-2

[VIEW COMPONENTS](#)



### ANGULATED MULTI-UNIT 20°


GH (mm)	ENGAGING
2,5/3,9	48.312.207.02-2
3,5/4,9	48.312.207.03-2
4,5/5,9	48.312.207.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH O222

LIST OF COMPATIBILITIES **AVAILABLE**  
MEGAGEN

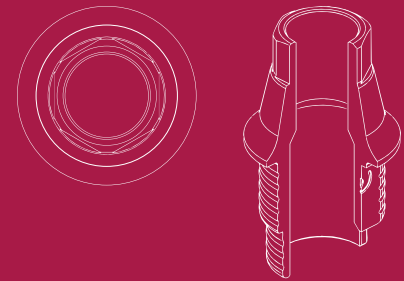

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	30°	-	31.320.222.01-2	31.310.222.01-2
2	25°	-	31.320.222.02-2	31.310.222.02-2
3	20°	-	31.320.222.03-2	31.310.222.03-2



### LAB SCANBODY

30.410.006.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.315.604.01-2
4	25°	33.415.604.01-2
6		33.615.604.01-2

## ANALOG

### DIGITAL ANALOG

34.610.222.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.222.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.078.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH O223

## LIST OF COMPATIBILITIES AVAILABLE

MEGAGEN

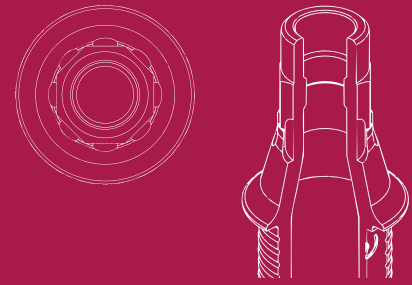

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	30°	-	31.323.223.01-2	31.313.223.01-2
2	25°	15°	31.323.223.02-2	31.313.223.02-2
3	20°	10°	31.323.223.03-2	31.313.223.03-2



#### LAB SCANBODY

30.413.002.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL
3		33.315.604.01-2
4	25°	33.415.604.01-2
6		33.615.604.01-2

### ANALOG

#### DIGITAL ANALOG

34.613.223.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.223.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.078.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH O229

## LIST OF COMPATIBILITIES AVAILABLE

PALTOP

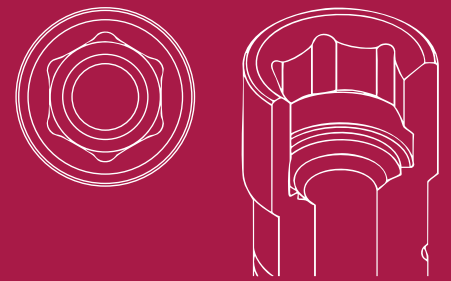

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	40°	-	31.320.229.01-2	31.310.229.01-2



#### LAB SCANBODY

30.410.006.01-2



### SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.064.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O236

LIST OF COMPATIBILITIES **AVAILABLE**  
ROOT

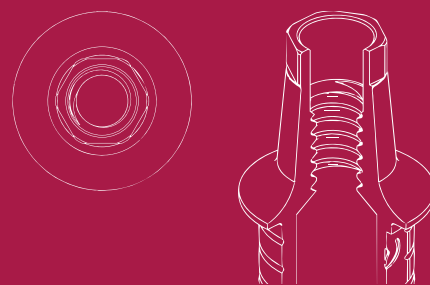

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	20°	25°	31.322.236.01-2	31.312.236.01-2



### LAB SCANBODY

30.412.001.01-2



## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.236.21-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

**SCREWS**


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.316.075.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



# COMPATIBLE WITH O242

## LIST OF COMPATIBILITIES AVAILABLE

OXY

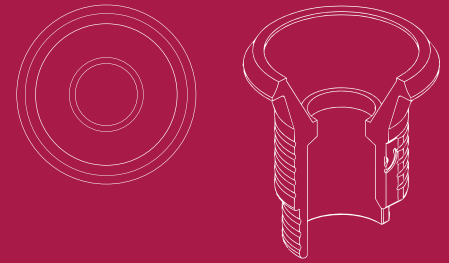

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	40°	-	31.323.242.01-2	-
<b>LAB SCANBODY</b>				
30.413.005.01-2				



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.370.716.01-2	34.613.242.01-2
4	25°	33.470.716.01-2	
6		33.670.716.01-2	



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
54.322.242.31-2	49.416.000.04-2	13	D	43.601.104.01-2
	49.416.000.05-2	13	E	
	<b>CAPS</b>	<b>HEIGHT</b>	<b>TYPE</b>	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



## SCREWS


DYNAMIC SCREW	DYNAMIC SCREW Ø2,6	LENGTH	SCREWDRIVER
		18	43.618.201.01-2
41.318.045.01-2	41.318.055.01-2 (Direct MU)	24	43.624.201.01-2
		32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm G<sub>s</sub> = Standard maximum angulation G<sub>z</sub> = Standard maximum angulation G<sub>d</sub> = Direct to implant maximum angulation

# COMPATIBLE WITH O243

LIST OF COMPATIBILITIES **AVAILABLE**  
GMI (ILERIMPLANT)

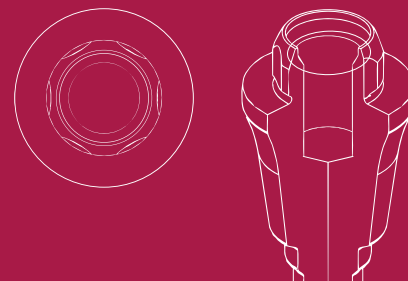

## SCREWS

DYNAMIC SCREW	LENTH	SCREWDRIVER
41.316.084.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.003.01-2	Hex. 1.20	43.601.103.02-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT


GH (mm)	NON ENGAGING
2	42.303.243.02-2
3	42.303.243.03-2

[VIEW COMPONENTS](#)



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH O245

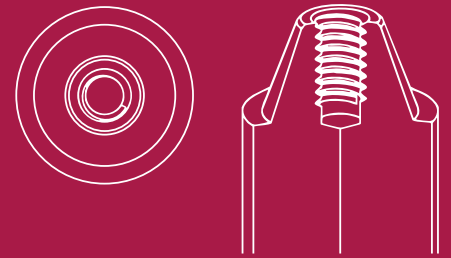

## LIST OF COMPATIBILITIES AVAILABLE

C-TECH

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,6	40°	-	31.323.245.01-2	-



LAB  
SCANBODY

---

30.413.005.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.039.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O246

## LIST OF COMPATIBILITIES AVAILABLE

C-TECH

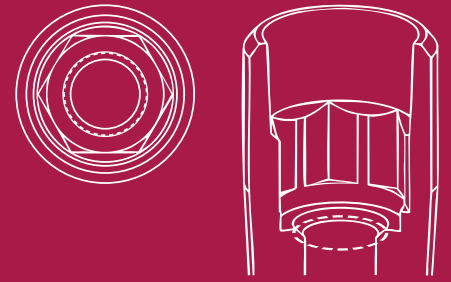

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	25°	-	31.322.246.01-2	31.312.246.01-2
2	25°	-	31.322.246.02-2	31.312.246.02-2
<b>LAB SCANBODY</b>				
30.412.001.01-2				



### SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.318.080.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O247

LIST OF COMPATIBILITIES **AVAILABLE**  
DIO IMPLANTS

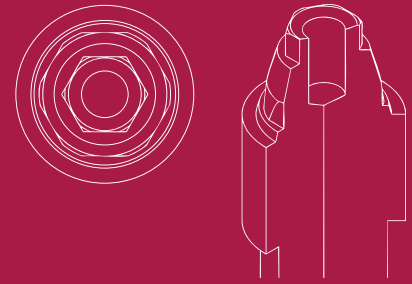

## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	40°	-	31.323.247.01-2	-
<b>LAB SCANBODY</b>				
30.413.005.01-2				



**LIBRARY OPTIONS:** GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.322.247.31-2	49.414.000.01-2	6	A	43.601.103.02-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		
	CAPS	HEIGHT	TYPE	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.040.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm G1 = Standard maximum angulation G2 = Standard maximum angulation G3 = Direct to implant maximum angulation

# COMPATIBLE WITH O249

LIST OF COMPATIBILITIES **AVAILABLE**  
MEDENTIS

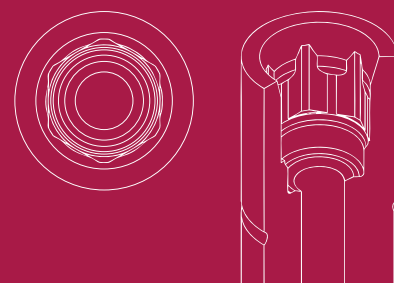


## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	40°	-	31.320.249.01-2	31.310.249.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.128.01-2	50.310.249.03-2 (IG=3mm)	43.621.415.01-2



### LAB SCANBODY

30.410.006.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.315.804.01-2	34.610.249.01-2
4	25°	33.415.804.01-2	
6		33.615.804.01-2	

## ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCREWS


DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43,618.201.01-2
41.314.080.01-2	24	43,624.201.01-2
	32	43,632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.003.08-2	Hex 1,20	43,601.103.02-2



# COMPATIBLE WITH O251

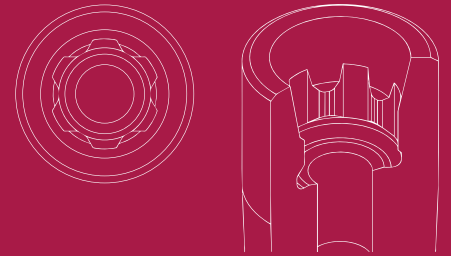

## LIST OF COMPATIBILITIES AVAILABLE

BREXENT MEDICAL

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1	40°	25°	31.322.251.01-2	31.312.251.01-2
1,5	40°	20°	31.322.251.02-2	31.312.251.02-2
3	25°	10°	31.322.251.04-2	31.312.251.04-2



#### LAB SCANBODY

30.412.001.01-2



### ANALOG

#### DIGITAL ANALOG

34.612.251.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.251.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.064.02-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.01-2	Hex 1,20	43.601.107.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.251.01-2
2	42.302.251.02-2
3	42.302.251.03-2
4	42.302.251.04-2

[VIEW COMPONENTS](#)




### INTERNAL MULTI-UNIT

GH (mm)	NON ENGAGING
3	62.302.251.03-2
4	62.302.251.04-2

[VIEW COMPONENTS](#)



# COMPATIBLE WITH O257

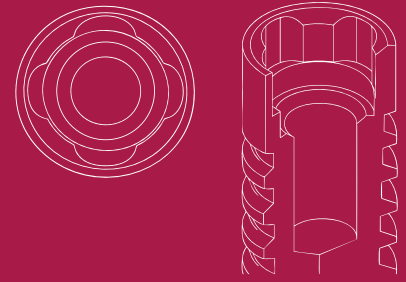

## LIST OF COMPATIBILITIES AVAILABLE

BTI

### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.318.065.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.318.003.01-2	Hex. 1.20	43.601.103.02-2



### MULTI-UNIT

#### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.257.01-2
2	42.302.257.02-2
3	42.302.257.03-2
4	42.302.257.04-2

[VIEW COMPONENTS](#)




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH O258

## LIST OF COMPATIBILITIES AVAILABLE

ASTRA

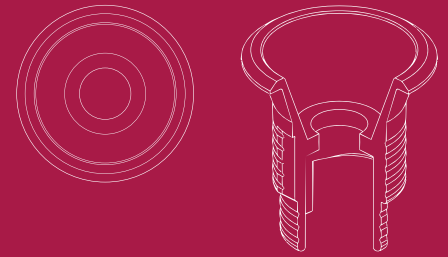

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,3	45°	30°	31.323.025.01-2	-



### DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$ CH=5mm	$\alpha_s$ CH=7mm	$\alpha_s$ CH=9mm	NON ENGAGING	ENGAGING
0,3	30°	25°	10°	31.323.025.21-2	-



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
8	52.408.112.01-2	50.313.025.02-2	43.621.410.01-2
10	52.410.111.01-2	50.313.025.01-2	43.624.410.01-2 43.620.411.01-2



LAB SCANBODY	MINI SCANBODY	SCANALOG
30.413.005.01-2	53.413.025.01-2	23.413.025.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

## DYNAMIC MILLING TOOL

## ANALOG

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG	ANALOG
3		33.390.716.01-2	34.613.025.01-2	22.613.025.01-2
4	30°	33.490.716.01-2		
6		33.690.716.01-2		



## SCANBODY REFERENCE

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
	49.414.000.01-2	6	A	
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
54.322.025.31-2	49.416.000.05-2	13	E	43.625.108.01-2
	<b>CAPS</b>	<b>HEIGHT</b>	<b>TYPE</b>	
	49.418.000.01-2	3,8	Regular	
	49.418.000.02-2	3,8	Wide	
	49.419.000.01-2	6	Regular	
	49.419.000.02-2	6	Wide	
	49.420.000.01-2	8	Regular	
	49.420.000.02-2	8	Wide	



**SCREWS**

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.039.01-2	24	43.624.201.01-2
	32	43.632.201.01-2




STRAIGHT SCREW	TYPE	SCREWDRIVER
40.314.005.04-2	Hex 1,27	43.625.105.01-2



# COMPATIBLE WITH O260

LIST OF COMPATIBILITIES **AVAILABLE**  
STRAUMANN

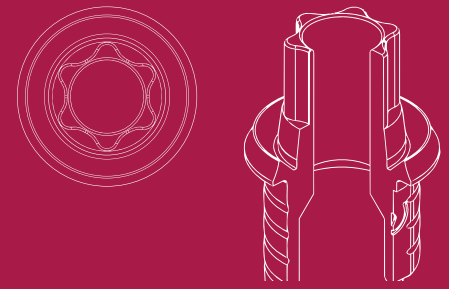


## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	40°	-	31.320.260.01-2	31.310.260.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.310.207.03-2 (IG=3mm)	43.621.410.01-2
12	52.412.103.01-2		43.624.410.01-2



LAB SCANBODY	SCANALOG
30.410.006.01-2	23.410.260.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2	34.610.260.01-2
4	30°	33.445.856.01-2	
6		33.645.856.01-2	



## ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.207.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.066.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.03-2	TORX T6	43.601.107.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT


GH (mm)	NON ENGAGING
1	42.302.207.01-2
2	42.302.207.02-2
3	42.302.207.03-2
4	42.302.207.04-2



[VIEW COMPONENTS](#)

# COMPATIBLE WITH O261

LIST OF COMPATIBILITIES **AVAILABLE**  
STRAUMANN

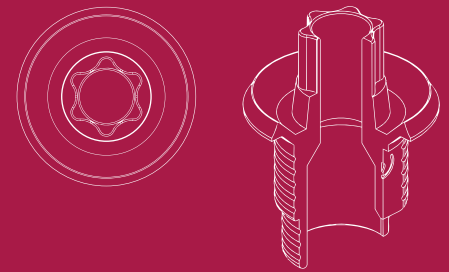


## STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	40°	-	31.323.261.01-2	31.313.261.01-2



## DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.310.207.03-2 (IG=3mm)	43.621.410.01-2
12	52.412.103.01-2		43.624.410.01-2



LAB SCANBODY	SCANALOG
30.413.004.01-2	23.413.261.01-2



## DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2	34.613.261.01-2
4	30°	33.445.856.01-2	
6		33.645.856.01-2	



## ANALOG

LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.207.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.066.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.03-2	TORX T6	43.601.107.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.207.01-2
2	42.302.207.02-2
3	42.302.207.03-2
4	42.302.207.04-2


[VIEW COMPONENTS](#)



# COMPATIBLE WITH O262

## LIST OF COMPATIBILITIES AVAILABLE

STRAUMANN

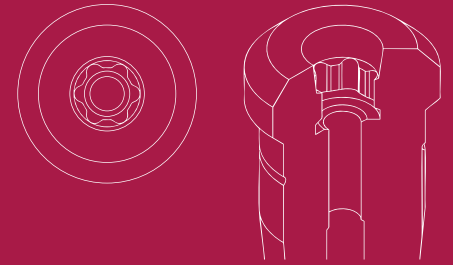


### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	40°	-	31.324.262.01-2	31.314.262.01-2



### DYNAMIC SCANBODY (LAB/CLIN)

H (mm)	SCANBODY	ADAPTOR	SCREWDRIVER ADAPTOR
10	52.410.103.01-2	50.310.207.03-2 (IG=3mm)	43.621.410.01-2
12	52.412.103.01-2		43.624.410.01-2



#### LAB SCANBODY

30.414.008.01-2



### DYNAMIC MILLING TOOL

SHANK	$\alpha_{di}$	DYNAMIC MILLING TOOL	DIGITAL ANALOG
3		33.345.856.01-2	34.614.262.01-2
4	30°	33.445.856.01-2	
6		33.645.856.01-2	

### ANALOG



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_{di}$  = Direct to implant maximum angulation

## SCANBODY OP

SCANBODY	PEEK PINS	HEIGHT	TYPE	SCREWDRIVER
54.315.207.21-2	49.414.000.01-2	6	A	43.601.107.01-2
	49.415.000.01-2	9	A	
	49.416.000.01-2	13	A	
	49.414.000.02-2	6	B	
	49.415.000.02-2	9	B	
	49.416.000.02-2	13	B	
	49.414.000.03-2	6	C	
	49.415.000.03-2	9	C	
	49.416.000.03-2	13	C	
	49.416.000.04-2	13	D	
49.416.000.05-2	13	E		



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.316.066.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



STRAIGHT SCREW	TYPE	SCREWDRIVER
40.316.007.03-2	TORX T6	43.601.107.01-2



## MULTI-UNIT

### STRAIGHT MULTI-UNIT

GH (mm)	NON ENGAGING
1	42.302.207.01-2
2	42.302.207.02-2
3	42.302.207.03-2
4	42.302.207.04-2


[VIEW COMPONENTS](#)



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm Gs = Standard maximum angulation Gc = Standard maximum angulation Gd = Direct to implant maximum angulation

# COMPATIBLE WITH O264

LIST OF COMPATIBILITIES **AVAILABLE**  
MEGAGEN

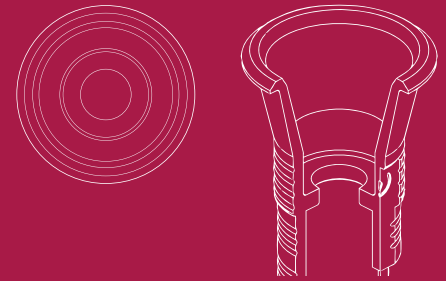

## DYNAMIC 3TIBASE

GH (mm)	$\alpha_s$	$\alpha_s$	$\alpha_s$	NON ENGAGING	ENGAGING
	CH=5mm	CH=7mm	CH=9mm		
0.3	-	25°	25°	31.323.264.21-2	-



### MINI SCANBODY

53.413.264.01-2



## SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.314.044.02-2	24	43.624.201.01-2
	32	43.632.201.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O265

## LIST OF COMPATIBILITIES AVAILABLE

ALPHA-DENT - PROTEG IMPLANTS

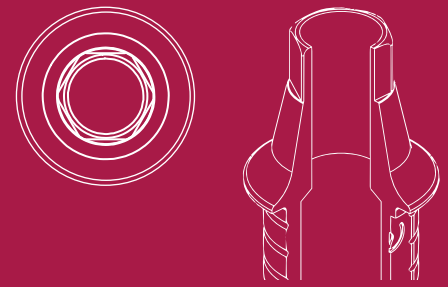

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
1,5	35°	-	31.322.265.03-2	31.312.265.03-2
2	25°	-	31.322.265.04-2	31.312.265.04-2



#### LAB SCANBODY

30.412.001.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.318.079.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O266



## LIST OF COMPATIBILITIES AVAILABLE

TBR

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	35°	-	31.320.266.01-2	31.310.266.01-2
2	25°	-	31.320.266.04-2	31.310.266.04-2



#### LAB SCANBODY

30.410.006.01-2



### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.068.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2




LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O267

## LIST OF COMPATIBILITIES AVAILABLE

TBR

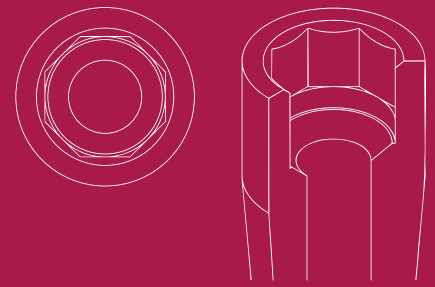

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	40°	-	31.322.267.01-2	31.312.267.01-2



#### LAB SCANBODY

30.412.001.01-2




### SCREWS

DYNAMIC SCREW	LENGTH	SCREWDRIVER
	18	43.618.201.01-2
41.320.068.01-2	24	43.624.201.01-2
	32	43.632.201.01-2



LIBRARY OPTIONS: GH = Gingival Height CH = Cement Height H = Height IG = Adaptor 3mm  $\alpha_s$  = Standard maximum angulation  $\alpha_c$  = Standard maximum angulation  $\alpha_d$  = Direct to implant maximum angulation

# COMPATIBLE WITH O268

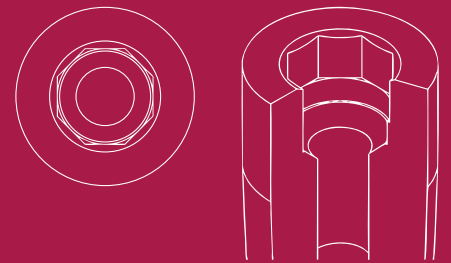

## LIST OF COMPATIBILITIES AVAILABLE

TBR

### STANDARD DYNAMIC TIBASE

GH (mm)	$\alpha_s$	$\alpha_c$	NON ENGAGING	ENGAGING
0,5	45°	-	31.323.268.01-2	31.313.268.01-2



#### LAB SCANBODY


30.413.002.01-2




### SCREWS



DYNAMIC SCREW	LENGTH	SCREWDRIVER
41.320.068.01-2	18	43.618.201.01-2
	24	43.624.201.01-2
	32	43.632.201.01-2



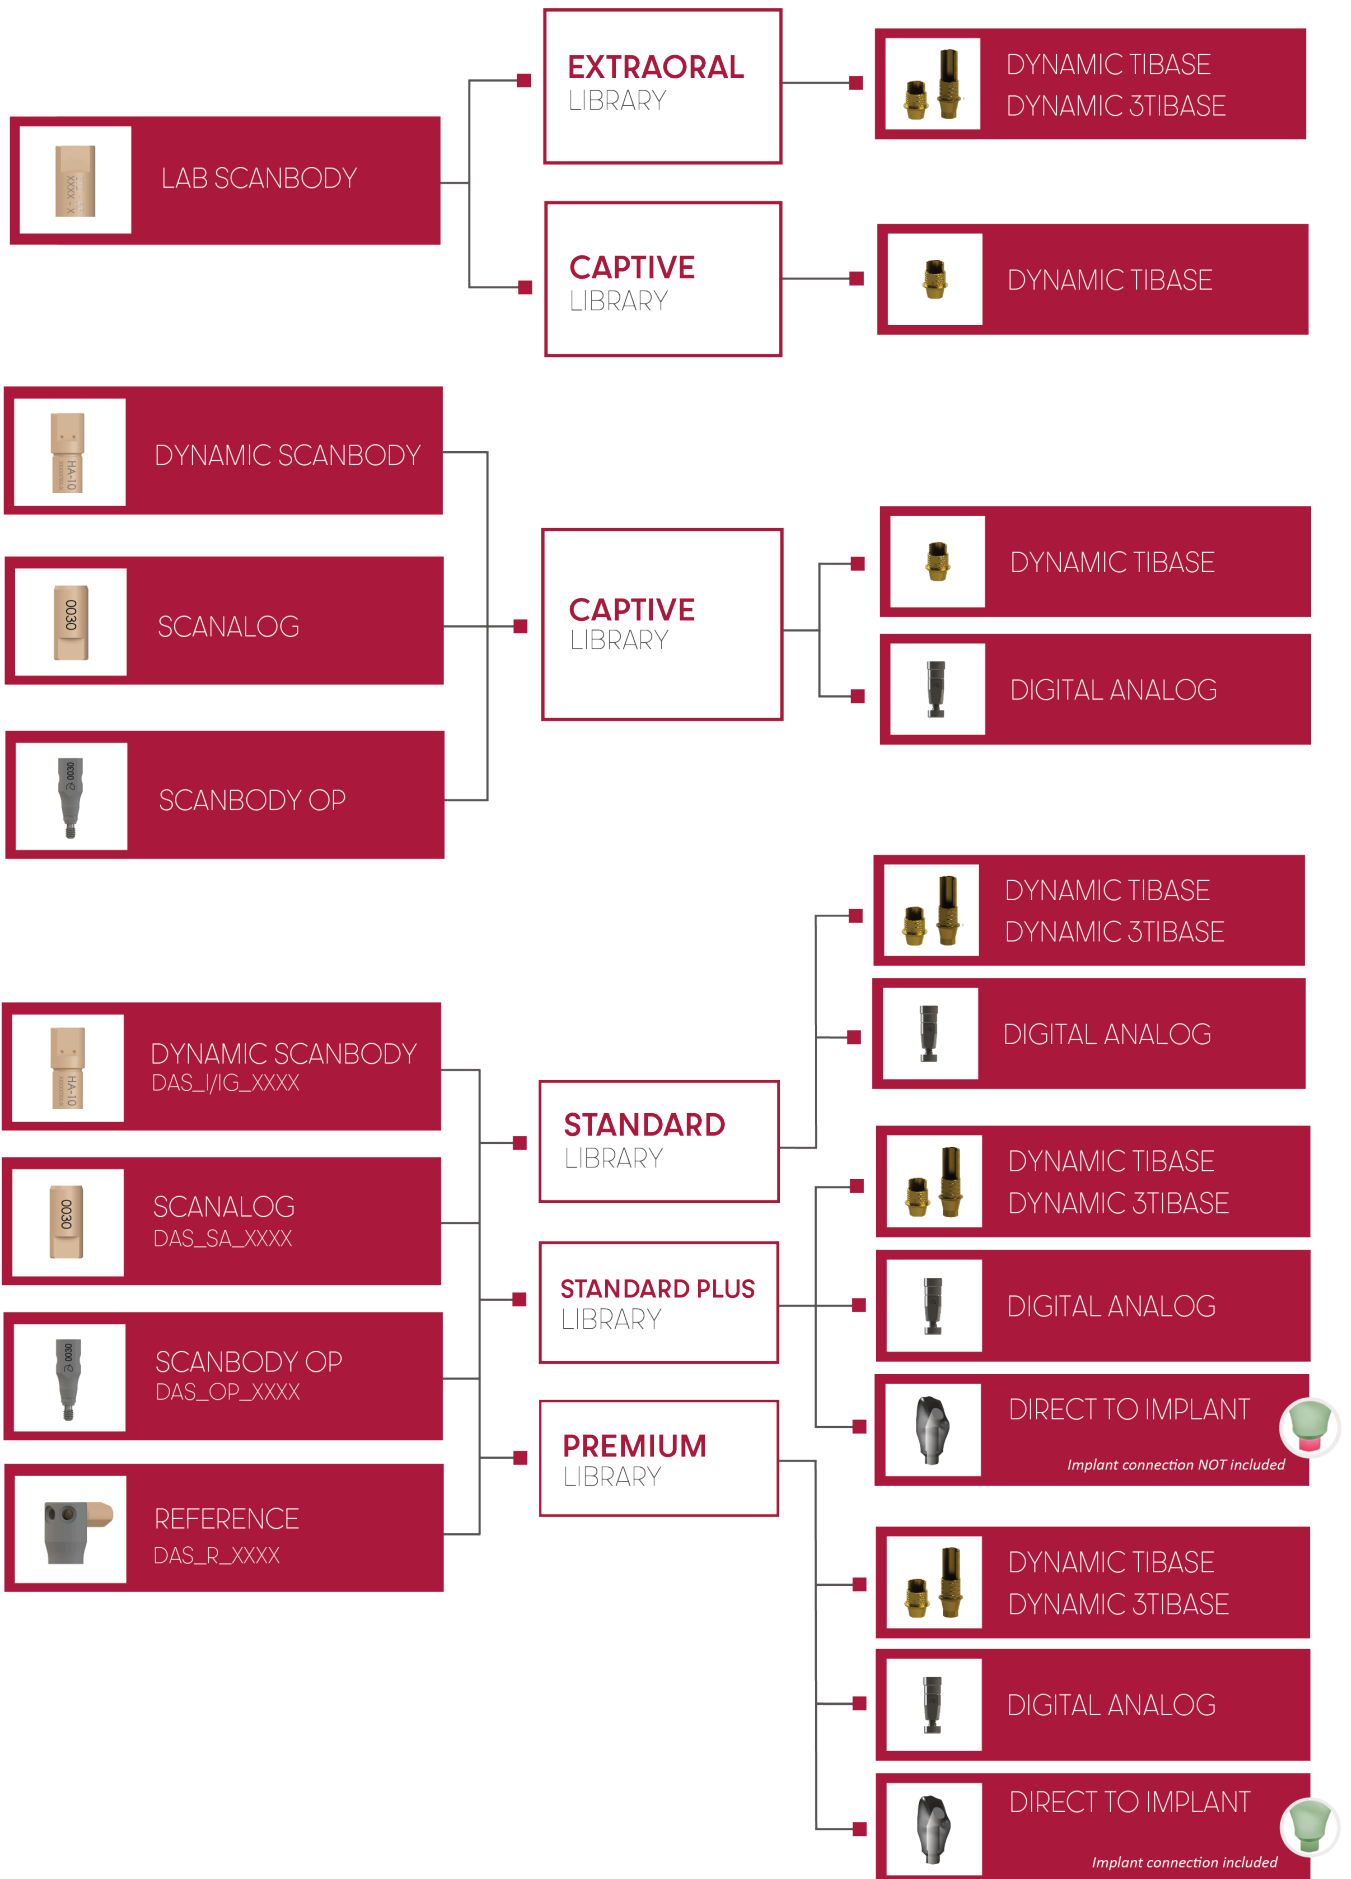

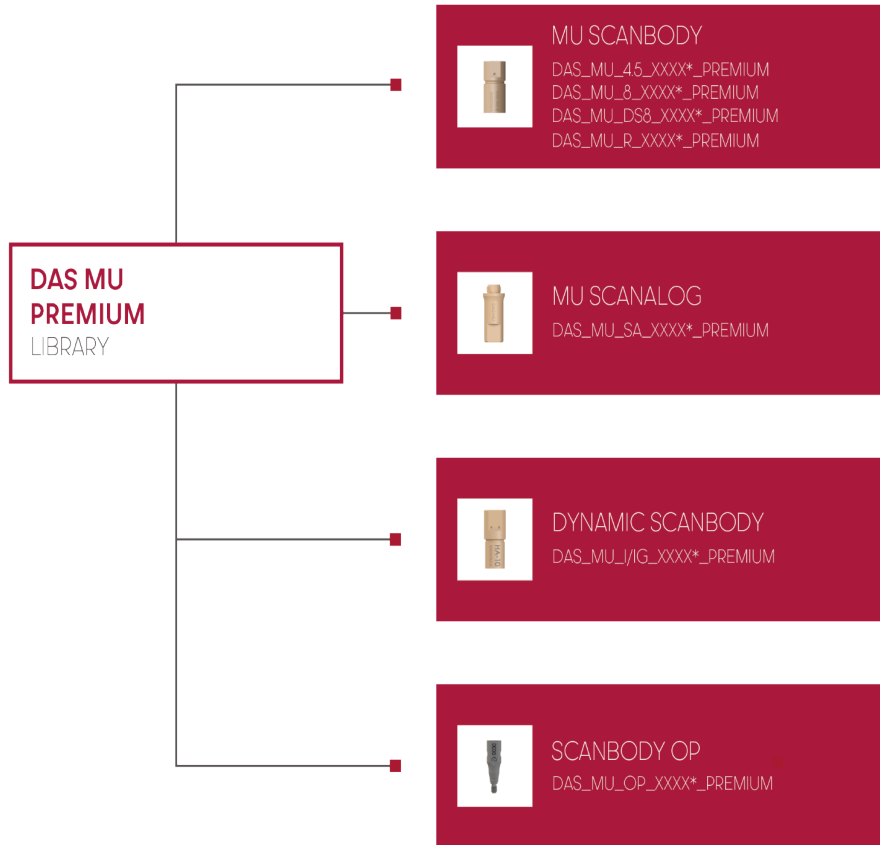

**DYNAMIC SCREWS** TECHNICAL SPECIFICATIONS  
**STRAIGHT SCREWS** TECHNICAL SPECIFICATIONS

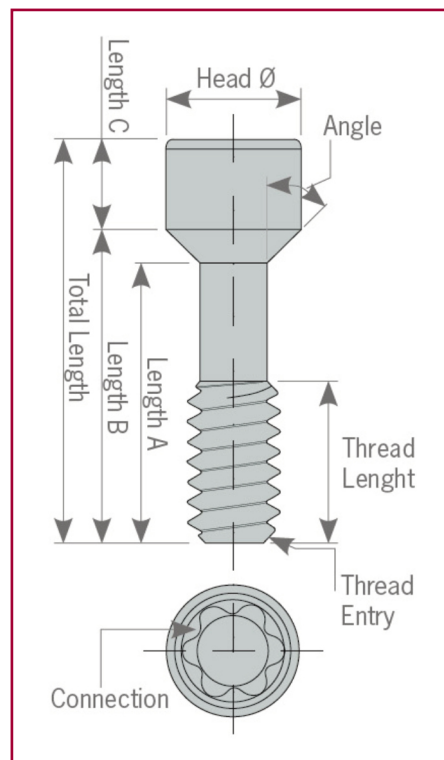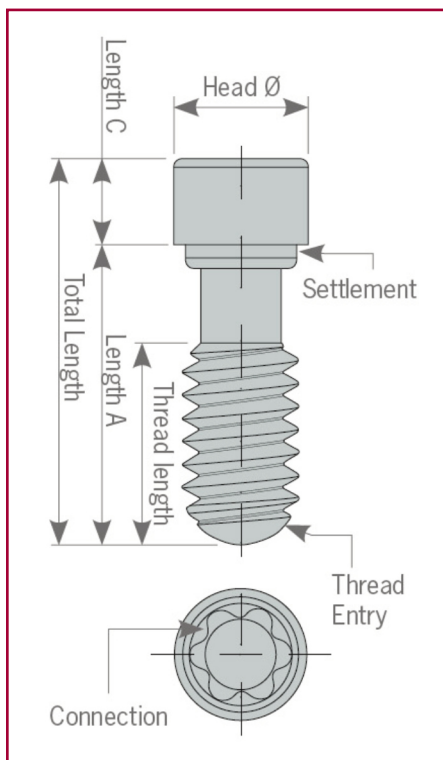

# DYNAMIC SCREWS TECHNICAL SPECIFICATIONS



REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.314.039.01-2	1.4	15 Ncm	3.9	1.8	2.1	-	1.8	2.4	straight	-	45° Chamfer	Hexalobular 1.70
41.314.040.02-2	1.4	15 Ncm	4	1.7	2.25	2.7	1.3	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.314.043.01-2	1.4	15 Ncm	4.3	1.8	2.03	2.9	1.4	2.3	conical	35°	45° Chamfer	Hexalobular 1.70
41.314.044.01-2	1.4	15 Ncm	4.4	2.15	2.73	3	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.314.046.01-2	1.4	15 Ncm	4.6	2.5	2.5	3.17	1.43	2.3	conical	35°	45° Chamfer	Hexalobular 1.70
41.314.064.01-2	1.4	15 Ncm	6.4	2.2	4.21	5.15	1.25	2.3	conical	25°	45° Chamfer	Hexalobular 1.70
41.314.067.02-2	1.4	15 Ncm	6.7	2.5	4.71	5.5	1.2	2.3	conical	35°	45° Chamfer	Hexalobular 1.70
41.314.070.01-2	1.4	15 Ncm	7	2.3	5.39	5.65	1.35	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.314.074.01-2	1.4	15 Ncm	7.4	3.55	5	5.99	1.41	2.3	conical	25°	45° Chamfer	Hexalobular 1.70
41.314.076.01-2	1.4	15 Ncm	7.6	2.4	5.88	6.35	1.25	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.314.080.01-2	1.4	15 Ncm	8	2.1	4.96	6.8	1.2	2.3	conical	15°	45° Chamfer	Hexalobular 1.70
41.314.084.01-2	1.4	15 Ncm	8.4	2.5	5.92	6.85	1.55	2.3	conical	35°	45° Chamfer	Hexalobular 1.70
41.314.105.01-2	1.4	15 Ncm	10.5	2.31	5	5.45	5.05	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.315.078.01-2	No-80	15 Ncm	7.8	2.45	5.77	6	1.8	2.3	conical	65°	45° Chamfer	Hexalobular 1.70
41.316.040.01-2	1.6	20 Ncm	4	2.07	2.3	2.47	1.53	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.316.048.01-2	1.6	20 Ncm	4.8	2.6	2.93	3.5	1.3	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.316.048.02-2	1.6	20 Ncm	4.8	2.85	3	3.58	1.22	2.3	conical	31°	45° Chamfer	Hexalobular 1.70
41.316.064.01-2	1.6	20 Ncm	6.4	3.15	4.7	5	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.316.064.02-2	1.6	20 Ncm	6.4	1.6	4.08	5.48	0.92	2.3	conical	15°	45° Chamfer	Hexalobular 1.70
41.316.066.01-2	1.6	20 Ncm	6.6	1.95	4.78	5.2	1.4	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.316.071.01-2	1.6	20 Ncm	7.1	2.8	5.2	5.54	1.56	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.316.072.01-2	1.6	20 Ncm	7.2	3.5	5.2	5.82	1.38	2.3	conical	30°	45° Chamfer	Hexalobular 1.70
41.316.073.01-2	1.6	20 Ncm	7.3	2.2	4.71	5.56	1.74	2.3	conical	35°	45° Chamfer	Hexalobular 1.70
41.316.076.01-2	1.6	20 Ncm	7.6	3.5	6.1	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.316.078.01-2	1.6	20 Ncm	7.84	2.2	5.51	7.04	0.8	2.3	conical	15°	45° Chamfer	Hexalobular 1.70
41.316.079.01-2	1.6	20 Ncm	7.9	2.30	5.42	6.60	1.3	2.3	conical	20°	45° Chamfer	Hexalobular 1.70
41.316.080.01-2	1.6	20 Ncm	8	3	6.3	6.51	1.49	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.316.081.01-2	1.6	20 Ncm	8.1	3	6.35	6.73	1.37	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.316.084.01-2	1.6	20 Ncm	8.4	3.5	6.8	-	1.6	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.316.084.02-2	1.6	20 Ncm	8.4	2.7	5.85	6.85	1.55	2.3	conical	30°	45° Chamfer	Hexalobular 1.70
41.316.086.01-2	1.6	20 Ncm	8.6	3	7.2	-	1.4	2.3	straight	-	45° Chamfer	Hexalobular 1.70
41.316.094.01-2	1.6	20 Ncm	9.4	2.9	7.62	8	1.4	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.316.108.01-2	1.6	20 Ncm	10.8	2.2	4.72	5.56	5.24	2.3	conical	35°	45° Chamfer	Hexalobular 1.70
41.316.115.01-2	1.6	20 Ncm	11.5	3.5	5.2	5.82	5.68	2.3	conical	30°	45° Chamfer	Hexalobular 1.70
41.316.118.01-2	1.6	20 Ncm	11.8	3.5	6.1	-	5.7	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.316.124.01-2	1.6	20 Ncm	12.4	2.2	5.55	7.05	5.35	2.3	conical	15°	45° Chamfer	Hexalobular 1.70
41.316.132.01-2	1.6	20 Ncm	13.2	2.9	7.63	8	5.2	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.317.040.01-2	N1-72	25 Ncm	4	2.1	2.5	-	1.5	2.3	straight	-	45° Chamfer	Hexalobular 1.70
41.317.041.01-2	N1-72	25Ncm	4.1	1.9	2.3	2.47	1.63	2.3	conical	55°	45° Chamfer	Hexalobular 1.70
41.317.065.01-2	N1-72	25 Ncm	6.5	2.4	4.7	5.18	1.33	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.317.073.01-2	N1-72	25 Ncm	7.3	2.5	5.5	5.77	1.53	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.317.106.01-2	N1-72	25 Ncm	10.6	2.8	5.54	5.65	4.95	2.3	conical	70°	Semi-sphere	Hexalobular 1.70
41.318.043.01-2	1.8	25 Ncm	4.3	2	2.52	2.7	1.6	2.3	conical	55°	45° Chamfer	Hexalobular 1.70
41.318.044.01-2	1.8	25 Ncm	4.4	2.75	3	-	1.4	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.318.045.01-2	1.8	25 Ncm	4.5	2.3	2.81	2.9	1.6	2.3	conical	70°	45° Chamfer	Hexalobular 1.70
41.318.051.01-2	1.8	25 Ncm	5.1	2.7	3.55	3.7	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.318.064.01-2	1.8	25 Ncm	6.4	3.45	4.7	5.1	1.3	2.3	conical	35°	45° Chamfer	Hexalobular 1.70
41.318.065.01-2	1.8	25 Ncm	6.5	2.83	5	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.318.067.01-2	1.8	25 Ncm	6.7	2.35	4.93	5.4	1.3	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.318.068.01-2	1.8	25 Ncm	6.8	4	5.25	5.4	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.318.071.01-2	1.8	25 Ncm	7.1	2.6	5.54	5.65	1.45	2.3	conical	70°	45° Chamfer	Hexalobular 1.70
41.318.074.01-2	1.8	25 Ncm	7.4	3.8	5.8	6.04	1.36	2.3	conical	50°	45° Chamfer	Hexalobular 1.70
41.318.075.01-2	1.8	25 Ncm	7.5	3.3	6.1	-	1.4	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.318.076.01-2	1.8	25 Ncm	7.6	2.52	5.73	6.2	1.4	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.318.077.01-2	1.8	25 Ncm	7.7	2.5	5.59	6.5	1.2	2.3	conical	30°	45° Chamfer	Hexalobular 1.70
41.318.077.02-2	1.8	25 Ncm	7.7	2.2	6.08	6.35	1.35	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.318.080.01-2	1.8	25 Ncm	8	4	6.5	-	1.5	2.3	straight	-	45° Chamfer	Hexalobular 1.70
41.318.083.01-2	1.8	25 Ncm	8.3	4.25	6.79	6.95	1.35	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.320.048.01-2	2	25 Ncm	4.8	2.7	3.3	3.4	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.320.051.01-2	2	25 Ncm	5.1	3.1	3.6	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.060.01-2	2	25 Ncm	6	2.7	4.5	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.065.01-2	2	25 Ncm	6.5	2.7	5	-	1.5	2.3	straight	-	45° Chamfer	Hexalobular 1.70
41.320.068.01-2	2	25 Ncm	6.8	4.4	5.3	5.4	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.320.090.01-2	2	25 Ncm	9	4	7.5	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.094.01-2	2	25 Ncm	9.4	3	7.84	8	1.4	2.3	conical	45°	45° Chamfer	Hexalobular 1.70

# DYNAMIC SCREWS TECHNICAL SPECIFICATIONS



REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.320.117.01-2	2	25 N·cm	11.7	2.75	5.91	6.18	5.52	2.3	conical	35°	Semi-sphere	Hexalobular 1.70
41.320.125.01-2	2	25 N·cm	12.5	3.3	6.33	6.5	6	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.320.129.01-2	2	25 N·cm	12.9	4.7	6.7	-	6.2	2.4	straight	-	Semi-sphere	Hexalobular 1.70
41.320.137.01-2	2	25 N·cm	13.7	4	7.5	-	6.2	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.325.067.01-2	2.5	25 N·cm	6.7	4.6	5.1	-	1.6	2.85	straight	-	Semi-sphere	Hexalobular 1.70
41.318.051.01-2	1.8	25 N·cm	5.1	2.7	3.55	3.7	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.318.051.02-2	1.8	25 N·cm	5.1	2.7	3.38	3.65	1.45	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.318.064.01-2	1.8	25 N·cm	6.4	3.45	4.7	5.1	1.3	2.3	conical	35°	45° Chamfer	Hexalobular 1.70
41.318.067.01-2	1.8	25 N·cm	6.7	2.35	4.93	5.4	1.3	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.318.069.01-2	1.8	25 N·cm	6.9	3.5	5.4	-	1.5	2.3	straight	-	45° Chamfer	Hexalobular 1.70
41.318.070.01-2	1.8	25 N·cm	7	3.4	5.303	5.7	1.3	2.3	conical	-	45° Chamfer	Hexalobular 1.70
41.318.071.01-2	1.8	25 N·cm	7.1	2.6	5.54	5.65	1.45	2.3	conical	70°	45° Chamfer	Hexalobular 1.70
41.318.074.01-2	1.8	25 N·cm	7.4	3.8	5.8	6.04	1.36	2.3	conical	50°	45° Chamfer	Hexalobular 1.70
41.318.076.01-2	1.8	25 N·cm	7.6	2.52	5.73	6.2	1.4	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.318.077.01-2	1.8	25 N·cm	7.7	2.5	5.59	6.5	1.2	2.3	conical	30°	45° Chamfer	Hexalobular 1.70
41.318.079.01-2	1.8	25 N·cm	7.9	4	6.34	6.5	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.318.080.01-2	1.8	25 N·cm	8	4	6.5	-	1.5	2.3	straight	-	45° Chamfer	Hexalobular 1.70
41.318.083.01-2	1.8	25 N·cm	8.3	4.25	6.79	6.95	1.35	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.318.111.01-2	1.8	25 N·cm	11.1	2.2	6.06	6.35	4.75	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.318.122.01-2	1.8	25 N·cm	12.2	3.8	5.8	6	6.2	2.3	conical	50°	45° Chamfer	Hexalobular 1.70
41.320.038.01-2	2	25 N·cm	3.81	2.35	2.35	2.42	1.39	2.35	conical	70°	45° Chamfer	Hexalobular 1.70
41.320.039.01-2	2	25 N·cm	3.9	1.9	2.41	2.5	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.320.042.01-2	2	25 N·cm	4.2	2.2	3.1	-	1.1	2.315	straight	-	30° Chamfer	Hexalobular 1.70
41.320.043.01-2	2	25 N·cm	4.3	2	2.5	-	1.8	2.3	straight	-	45° Chamfer	Hexalobular 1.70
41.320.044.01-2	2	25 N·cm	4.4	2.45	2.95	3.1	1.3	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.320.047.01-2	2	25 N·cm	4.7	3	3.3	-	1.4	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.048.01-2	2	25 N·cm	4.8	2.7	3.3	3.4	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.320.050.01-2	2	25 N·cm	5	2.8	3.35	3.6	1.4	2.3	conical	31°	Semi-sphere	Hexalobular 1.70
41.320.050.02-2	2	25 N·cm	5	3	3.5	-	1.5	1.5	straight	-	45° Chamfer	Hexalobular 1.70
41.320.051.01-2	2	25 N·cm	5.1	3.1	3.6	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.052.01-2	2	25 N·cm	5.2	3	3.7	-	1.5	2.6	straight	-	30° Chamfer	Hexalobular 1.70
41.320.060.01-2	2	25 N·cm	6	2.7	4.5	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.065.01-2	2	25 N·cm	6.5	2.7	5	-	1.5	2.3	straight	-	45° Chamfer	Hexalobular 1.70
41.320.067.01-2	2	25 N·cm	6.7	2.3	3.59	5.7	1	2.58	conical	15°	45° Chamfer	Hexalobular 1.70
41.320.068.01-2	2	25 N·cm	6.8	4.4	5.3	5.4	1.4	2.3	conical	60°	45° Chamfer	Hexalobular 1.70
41.320.070.01-2	2	25 N·cm	7	3	5.6	-	1.4	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.071.01-2	2	25 N·cm	7.1	4	5.11	5.55	1.55	2.3	conical	20°	45° Chamfer	Hexalobular 1.70
41.320.074.01-2	2	25 N·cm	7.4	3.3	6	-	1.4	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.075.01-2	2	25 N·cm	7.5	2.75	5.9	6.19	1.31	2.3	conical	35°	Semi-sphere	Hexalobular 1.70
41.320.079.01-2	2	25 N·cm	7.9	3.3	6.32	6.5	1.4	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.320.081.01-2	2	25 N·cm	8.1	4.6	5.53	5.8	2.3	2.3	conical	65°	45° Chamfer	Hexalobular 1.70
41.320.082.01-2	2	25 N·cm	8.2	4.7	6.7	-	1.5	2.4	straight	-	Semi-sphere	Hexalobular 1.70
41.320.090.01-2	2	25 N·cm	9	4	7.5	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.094.01-2	2	25 N·cm	9.4	3	7.84	8	1.4	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.320.094.02-2	2	25 N·cm	9.4	3	7.9	-	1.5	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.320.117.01-2	2	25 N·cm	11.7	2.75	5.91	6.18	5.52	2.3	conical	35°	Semi-sphere	Hexalobular 1.70
41.320.125.01-2	2	25 N·cm	12.5	3.3	6.33	6.5	6	2.3	conical	45°	45° Chamfer	Hexalobular 1.70
41.320.129.01-2	2	25 N·cm	12.9	4.7	6.7	-	6.2	2.4	straight	-	Semi-sphere	Hexalobular 1.70
41.320.137.01-2	2	25 N·cm	13.7	4	7.5	-	6.2	2.3	straight	-	Semi-sphere	Hexalobular 1.70
41.325.054.01-2	2.5	25 N·cm	5.4	4.6	4.1	-	1.3	2.865	straight	-	Semi-sphere	Hexalobular 1.70
41.325.067.01-2	2.5	25 N·cm	6.7	4.6	5.1	-	1.6	2.85	straight	-	Semi-sphere	Hexalobular 1.70

# STRARICHT SCREWS TECHNICAL SPECIFICATIONS



REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.312.003.01-2	1.2	0.25	15 Ncm	7.85	2.7	6.2	6.55	1.3	1.9	conical	45° Chamfer	Hex. 1.20
40.314.003.01-2	1.4	0.3	15 Ncm	3.9	1.91	2.1	-	1.8	2.4	straight	45° Chamfer	Hex. 1.20
40.314.003.02-2	1.4	0.3	15 Ncm	4	2	2.2	-	1.8	2.3	straight	45° Chamfer	Hex. 1.20
40.314.003.03-2	1.4	0.3	15 Ncm	7.6	2.4	6.05	6.3	1.3	1.9	conical	45° Chamfer	Hex. 1.20
40.314.003.04-2	1.4	0.3	15 Ncm	7.5	2.5	5.45	5.7	1.8	1.85	conical	45° Chamfer	Hex. 1.20
40.314.003.05-2	1.4	0.3	15 Ncm	5.3	1.34	3.7	-	1.6	2.1	straight	30° Chamfer	Hex. 1.25
40.314.004.01-2	1.4	0.3	15 Ncm	6.3	2.2	4.6	5.1	1.2	2.1	conical	30° Chamfer	Hex. 1.25
40.314.005.01-2	1.4	0.3	15 Ncm	7.6	3.6	5.21	6	1.6	2.15	conical	45° Chamfer	Hex. 1.27
40.314.005.02-2	1.4	0.3	15 Ncm	7.5	2.4	5.5	5.7	1.8	2.1	conical	45° Chamfer	Hex. 1.27
40.314.005.04-2	1.4	0.3	15 Ncm	4	1.7	2.25	-	1.75	2.1	straight	45° Chamfer	Hex. 1.27
40.314.007.01-2	1.4	0.3	15 Ncm	4	1.8	2.01	2.8	1.2	2.2	conical	45° Chamfer	Torx T6
40.314.007.02-2	1.4	0.3	15 Ncm	7	2.1	6.2	2.25	0.8	2.1	conical	45° Chamfer	Torx T6
40.314.007.03-2	1.4	0.3	15 Ncm	5.1	1.1	3.35	3.9	1.2	2.1	conical	45° Chamfer	Torx T6
40.314.008.01-2	1.4	0.3	15 Ncm	3.6	1.8	2.1	-	1.5	2.1	straight	45° Chamfer	Unigrip
40.314.008.02-2	1.4	0.3	15 Ncm	6.7	2.5	4.87	5.3	1.4	1.8	conical	45° Chamfer	Unigrip
40.314.008.03-2	1.4	0.3	15 Ncm	6.65	1.6	3.65	5.75	0.9	2.95	conical	45° Chamfer	Unigrip
40.314.008.04-2	1.4	0.3	15 Ncm	4.8	1.1	3.05	3.6	1.2	2.1	conical	45° Chamfer	Unigrip
40.314.012.01-2	1.4	0.3	15 Ncm	4.5	1.7	2.01	2.4	2.1	2.15	conical	45° Chamfer	Star 1.50
40.314.014.01-2	1.4	0.3	15 Ncm	4.45	2.3	2.48	-	1.97	2.16	straight	45° Chamfer	Hex. 1.19
40.315.008.01-2	No-80	0.317	15 Ncm	8.3	2.45	5.79	5.95	2.35	2	conical	45° Chamfer	Unigrip
40.316.002.01-2	1.6	0.35	20 Ncm	7	2.79	4.86	5.44	1.56	2.3	conical	45° Chamfer	Cuad. 1.30
40.316.002.02-2	1.6	0.35	20 Ncm	9.3	3.3	7.3	-	2	2.3	straight	Semi-sphere	Cuad. 1.30
40.316.003.01-2	1.6	0.35	20 Ncm	8.4	2.5	6.6	-	1.8	2	straight	45° Chamfer	Hex. 1.20
40.316.003.02-2	1.6	0.35	20 Ncm	10.2	2	7.88	8.2	2	2.2	conical	45° Chamfer	Hex. 1.20
40.316.004.02-2	1.6	0.35	20 Ncm	8.8	3	6.73	7	1.8	2.1	conical	45° Chamfer	Hex. 1.25
40.316.004.03-2	1.6	0.35	20 Ncm	6.9	2.2	5.02	5.2	1.7	1.92	conical	45° Chamfer	Hex. 1.25
40.316.005.01-2	1.6	0.35	20 Ncm	7.5	3.6	5.44	5.9	1.6	2.13	conical	45° Chamfer	Hex. 1.27
40.316.005.02-2	1.6	0.35	20 Ncm	8.25	3	6.25	-	2	2.33	straight	45° Chamfer	Hex. 1.27
40.316.005.03-2	1.6	0.35	20 Ncm	8.25	3.03	6.25	-	2	2.45	straight	45° Chamfer	Hex. 1.27
40.316.005.04-2	1.6	0.35	20 Ncm	10.5	3.2	8.15	8.4	2.1	2.1	conical	45° Chamfer	Hex. 1.27
40.316.005.05-2	1.6	0.35	20 Ncm	7.6	2.7	5.21	5.5	2.1	2.1	conical	45° Chamfer	Hex. 1.27
40.316.005.06-2	1.6	0.35	20 Ncm	3.8	1.8	2.2	-	1.6	2.1	straight	45° Chamfer	Hex. 1.27
40.316.005.07-2	1.6	0.35	20 Ncm	8.8	2.85	6.73	6.9	1.9	2.15	conical	45° Chamfer	Hex. 1.27
40.316.005.08-2	1.6	0.35	20 Ncm	9	3.9	6.49	6.9	2.1	2.18	conical	45° Chamfer	Hex. 1.27
40.316.005.09-2	1.6	0.35	20 Ncm	8.5	1.6	6.46	7	1.5	2.2	conical	45° Chamfer	Hex. 1.27
40.316.007.01-2	1.6	0.35	20 Ncm	7.9	2	5.63	6.9	1	2.18	conical	45° Chamfer	Torx T6
40.316.007.02-2	1.6	0.35	20 Ncm	9	1.6	6.96	7.5	1.5	2.2	conical	45° Chamfer	Torx T6
40.316.008.02-2	1.6	0.35	20 Ncm	7.3	2.7	5.15	5.9	1.4	2.2	conical	45° Chamfer	Unigrip
40.316.008.03-2	1.6	0.35	20 Ncm	8.5	1.6	6.46	7	1.5	2.2	conical	45° Chamfer	Unigrip
40.316.012.01-2	1.6	0.35	20 Ncm	8	2.65	5.53	6	2	2.15	conical	45° Chamfer	Star 1.50
40.316.014.01-2	1.6	0.35	20 Ncm	7.9	2.3	5.42	6.46	1.44	2.2	conical	45° Chamfer	Hex. 1.19
40.317.002.01-2	N1-72	0.353	25 Ncm	8.17	3	5.31	5.87	2.3	2.4	conical	45° Chamfer	Cuad. 1.30
40.317.004.01-2	N1-72	0.353	25 Ncm	7.6	2.8	5.6	5.77	1.83	2.3	conical	45° Chamfer	Hex. 1.27
40.317.005.01-2	N1-72	0.353	25 Ncm	7.6	2.15	5.17	5.4	2.2	2.2	conical	45° Chamfer	Hex. 1.27
40.317.005.02-2	N1-72	0.353	25 Ncm	7.3	2.4	4.73	5.25	2.05	2.4	conical	45° Chamfer	Hex. 1.27
40.318.002.01-2	1.8	0.35	25 Ncm	7	3.2	5.2	-	1.8	2.5	straight	45° Chamfer	Cuad. 1.30
40.318.002.02-2	1.8	0.35	25 Ncm	8.3	2.6	6.6	-	1.7	2.45	straight	45° Chamfer	Cuad. 1.30
40.318.003.01-2	1.8	0.35	25 Ncm	6.8	3.3	5.2	-	1.6	2.3	straight	45° Chamfer	Hex. 1.20
40.318.003.02-2	1.8	0.35	25 Ncm	8	3.6	6	-	2	2.1	straight	45° Chamfer	Hex. 1.20
40.318.004.01-2	1.8	0.35	25 Ncm	7.2	4.8	5.36	5.9	1.3	2.4	conical	45° Chamfer	Hex. 1.25
40.318.004.02-2	1.8	0.35	25 Ncm	9.8	5.8	7.96	8.5	1.3	2.4	conical	45° Chamfer	Hex. 1.25
40.318.004.03-2	1.8	0.35	25 Ncm	7.65	3.3	5.17	5.75	1.9	2.4	conical	45° Chamfer	Hex. 1.25
40.318.005.01-2	1.8	0.35	25 Ncm	4.5	2.3	2.8	2.9	1.6	2.33	conical	45° Chamfer	Hex. 1.27
40.318.005.02-2	1.8	0.35	25 Ncm	7.6	3.6	5.76	6	1.6	2.33	conical	45° Chamfer	Hex. 1.27
40.318.005.03-2	1.8	0.35	25 Ncm	8.5	1.6	6.56	7	1.5	2.2	conical	45° Chamfer	Hex. 1.27
40.318.005.04-2	1.8	0.35	25 Ncm	5.2	1.6	3.41	3.8	1.4	2.2	conical	45° Chamfer	Hex. 1.27
40.318.006.01-2	1.8	0.35	25 Ncm	6	3	3.67	4	2	2.4	conical	45° Chamfer	Hex. 1.70
40.318.007.01-2	1.8	0.35	25 Ncm	9.1	4.25	7.32	7.45	1.65	2.18	conical	45° Chamfer	Torx T6
40.318.008.01-2	1.8	0.35	25 Ncm	8.3	2.5	6.5	-	1.8	2.45	straight	45° Chamfer	Unigrip
40.318.012.01-2	1.8	0.35	25 Ncm	7.25	2.4	4.93	5.25	2	2.15	conical	45° Chamfer	Star 1.50
40.318.012.02-2	1.8	0.35	25 Ncm	8	2.6	5.68	6	2	2.15	conical	45° Chamfer	Star 1.50

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.318.013.01-2	1.8	0.35	25 Ncm	7.7	2.5	5.7	6.4	1.3	2.2	conical	45° Chamfer	Hex. 1.00
40.320.002.01-2	2	0.4	30 Ncm	4.9	3.26	3.26	3.5	1.4	2.49	conical	45° Chamfer	Cuad. 1.30
40.320.002.02-2	2	0.4	30 Ncm	7.45	3	5.7	5.9	1.5	2.4	conical	45° Chamfer	Cuad. 1.30
40.320.002.03-2	2	0.4	30 Ncm	10.2	3.15	8.4	-	1.8	2.45	straight	45° Chamfer	Cuad. 1.30
40.320.003.01-2	2	0.4	30 Ncm	4.7	3	3.33	-	1.37	2.35	straight	45° Chamfer	Hex. 1.20
40.320.003.02-2	2	0.4	30 Ncm	7	3.25	5	-	2	2.4	straight	45° Chamfer	Hex. 1.20
40.320.003.03-2	2	0.4	30 Ncm	7.9	3.7	5.55	6.05	1.85	2.4	conical	45° Chamfer	Hex. 1.20
40.320.003.04-2	2	0.4	30 Ncm	8.4	2.75	5.68	6.35	2.05	2.3	conical	45° Chamfer	Hex. 1.20
40.320.003.05-2	2	0.4	30 Ncm	4.8	3.3	3.65	3.9	0.9	2.45	conical	45° Chamfer	Hex. 1.20
40.320.003.06-2	2	0.25	25 Ncm	4	2	2.5	-	1.5	2.3	straight	30° Chamfer	Hex. 1.20
40.320.003.07-2	2	0.25	25 Ncm	8.5	1.6	6.63	7	1.5	2.2	conical	45° Chamfer	Hex. 1.20
40.320.005.01-2	2	0.4	30 Ncm	7.6	3.7	6	-	1.6	2.33	straight	45° Chamfer	Hex. 1.27
40.320.005.02-2	2	0.4	30 Ncm	10.3	4	8.3	-	2	2.45	straight	45° Chamfer	Hex. 1.27
40.320.005.03-2	2	0.4	30 Ncm	10.3	3.5	8.3	-	2	2.33	straight	45° Chamfer	Hex. 1.27
40.320.005.04-2	2	0.4	30 Ncm	10.5	3.2	8.15	8.4	2.1	2.5	conical	45° Chamfer	Hex. 1.27
40.320.007.01-2	2	0.4	30 Ncm	6.7	2.25	3.59	5.7	1	2.58	conical	45° Chamfer	Torx T6
40.320.007.02-2	2	0.4	30 Ncm	7.4	3.3	6	-	1.4	2.3	straight	Semi-sphere	Torx T6
40.320.007.03-2	2	0.4	30 Ncm	7.4	2.8	5.9	6.1	1.3	2.4	conical	Semi-sphere	Torx T6
40.320.007.04-2	2	0.4	30 Ncm	4.6	2.96	3.21	3.5	1.1	2.45	conical	45° Chamfer	Torx T6
40.320.007.05-2	2	0.25	25 Ncm	5	3	3.5	-	1.5	2.6	straight	30° Chamfer	Torx T6
40.320.008.01-2	2	0.4	30 Ncm	7	3.25	5	-	2	2.4	straight	45° Chamfer	Unigrip
40.320.008.02-2	2	0.4	30 Ncm	7.3	3	5.8	6.2	1.1	2.5	conical	45° Chamfer	Unigrip
40.320.008.03-2	2	0.4	30 Ncm	10	3.1	8.5	-	1.5	2.45	straight	45° Chamfer	Unigrip
40.320.008.04-2	2	0.4	30 Ncm	8.5	1.6	6.63	7	1.5	2.2	conical	45° Chamfer	Unigrip
40.325.002.01-2	2.5	0.45	30 Ncm	7.41	3.5	4.75	5.29	2.12	2.87	conical	Semi-sphere	Cuad. 1.30
40.325.008.01-2	2.5	0.45	30 Ncm	7	2.8	5.6	-	1.4	3.4	straight	45° Chamfer	Unigrip
40.320.003.01-2	2	0.4	30 Ncm	4.7	3	3.33	-	1.37	2.35	straight	45° Chamfer	Hex. 1.20
40.320.003.02-2	2	0.4	30 Ncm	7	3.25	5	-	2	2.4	straight	45° Chamfer	Hex. 1.20
40.320.003.03-2	2	0.4	30 Ncm	7.9	3.7	5.55	6.05	1.85	2.4	conical	45° Chamfer	Hex. 1.20
40.320.003.04-2	2	0.4	30 Ncm	8.4	2.75	5.68	6.35	2.05	2.3	conical	45° Chamfer	Hex. 1.20
40.320.003.05-2	2	0.4	30 Ncm	4.8	3.3	3.65	3.9	0.9	2.45	conical	45° Chamfer	Hex. 1.20
40.320.003.06-2	2	0.25	25 Ncm	4	2	2.5	-	1.5	2.3	straight	30° Chamfer	Hex. 1.20
40.320.003.07-2	2	0.25	25 Ncm	8.5	1.6	6.63	7	1.5	2.2	conical	45° Chamfer	Hex. 1.20
40.320.003.08-2	2	0.4	25 Ncm	4.2	2.2	2.7	-	1.5	2.3	straight	30° Chamfer	Hex. 1.20
40.320.005.01-2	2	0.4	30 Ncm	7.6	3.7	6	-	1.6	2.33	straight	45° Chamfer	Hex. 1.27
40.320.005.02-2	2	0.4	30 Ncm	10.3	4	8.3	-	2	2.45	straight	45° Chamfer	Hex. 1.27
40.320.005.03-2	2	0.4	30 Ncm	10.3	3.5	8.3	-	2	2.33	straight	45° Chamfer	Hex. 1.27
40.320.005.04-2	2	0.4	30 Ncm	10.5	3.2	8.15	8.4	2.1	2.5	conical	45° Chamfer	Hex. 1.27
40.320.005.05-2	2	0.4	25 Ncm	9	2.15	6.93	7.3	1.7	2.2	conical	45° Chamfer	Hex. 1.27

## SCREWDRIVERS



## STRAIGHT SCREWS

Straight screws cover all the thread metrics available on the market. We have several lengths for each metric to make the adaptation to the milled structures easier.




# DYNAMIC MILLING TOOL SPECIFICATIONS




MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		Øc		Lc	Lu	Øv	Øs	Lt
BEGO RS/RSX 3° ASTRA EVOLUTION 3.0° *Only for titanium and soft materials	33.325.472.01-2	1.4	25	0.4	4.7	0.5	3	50
	33.425.472.01-2	1.4	25	0.4	4.7	0.5	4	50
	33.625.472.01-2	1.4	25	0.4	4.7	0.5	6	50
STRAUMANN BONE LEVEL NP STRAUMANN BONE LEVEL RP MEDENTIS ICX TEMPLANT 4.1 STRAUMANN SYNOCTA 3.5 MEDENTIS ICX NARROW	33.315.804.01-2	1.6	15	0.7	8	0.65	3	50
	33.415.804.01-2	1.6	15	0.7	8	0.65	4	50
	33.615.804.01-2	1.6	15	0.7	8	0.65	6	50
ANTHOGYR AXIOM RG/PX XNP ANTHOGYR AXIOM RG/PX RP ANTHOGYR AXIOM RG/PX WP	33.320.704.01-2	1.6	20	0.7	7	0.8	3	50
	33.420.704.01-2	1.6	20	0.7	7	0.8	4	50
	33.620.704.01-2	1.6	20	0.7	7	0.8	6	50
ASTRA EVOLUTION 3.6 ANKYLOS ALPHABIO CONICAL STANDARD CONNECTION LASAK BIONIQ QR NEODENT GM ANKYLOS BALANCE BASE	33.330.734.01-2	1.6	30	0.7	7.3	0.8	3	50
	33.430.734.01-2	1.6	30	0.7	7.3	0.8	4	50
	33.630.734.01-2	1.6	30	0.7	7.3	0.8	6	50
NOBEL BIOCARE ACTIVE NP NOBEL BIOCARE ACTIVE 3.0 LASAK BIONIQ QN	33.335.754.01-2	1.6	35	0.7	7.5	0.65	0.5	50
	33.435.754.01-2	1.6	35	0.7	7.5	0.65	4	50
	33.635.754.01-2	1.6	35	0.7	7.5	0.65	6	50
OSSTEM TS NP CAMLOG SCREW LINE 3.8 NP CAMLOG SCREW LINE 4.3 RP KLOCKNER VEGA NV XIVE S 3.4 BIOTECH DENTAL KONTACT XNP BIOTECH DENTAL KONTACT RP DIO UF NP CAMLOG SCREW-LINE 3.3	33.345.804.01-2	1.6	45	0.7	8	0.65	3	50
	33.445.804.01-2	1.6	45	0.7	8	0.65	4	50
	33.645.804.01-2	1.6	45	0.7	8	0.65	6	50
MIS C1 NP MIS M4 NP CONELOG 3.8 CONELOG 4.3 ASTRA YELLOW ALPHABIO CONICAL HEX CONNECTION	33.360.754.01-2	1.6	60	0.7	7.5	0.65	3	50
	33.460.754.01-2	1.6	60	0.7	7.5	0.65	4	50
	33.660.754.01-2	1.6	60	0.7	7.5	0.65	6	50
BIOMET 3i CERTAIN NP ASTRA AQUA	33.390.754.01-2	1.6	90	0.7	7.5	0.65	3	50
	33.490.754.01-2	1.6	90	0.7	7.5	0.65	4	50
	33.690.754.01-2	1.6	90	0.7	7.5	0.65	6	50
ASTRA EVOLUTION 4.2	33.350.775.01-2	1.7	50	0.7	7.7	0.8	3	50
	33.450.775.01-2	1.7	50	0.7	7.7	0.8	4	50
	33.650.775.01-2	1.7	50	0.7	7.7	0.8	6	50
BIOMET 3i CERTAIN RP NOBEL BIOCARE BRANEMARK NP NOBEL BIOCARE REPLACE NP MEGAGEN ANYRIDGE RP BIOMET 3i CERTAIN WP	33.390.805.01-2	1.7	90	0.7	8	0.65	3	50
	33.490.805.01-2	1.7	90	0.7	8	0.65	4	50
	33.690.805.01-2	1.7	90	0.7	8	0.65	6	50
*BEGO S/RI 3.25-3.75 BEGO S/RI 4.1 BEGO S/RI 4.5 BEGO S/RI 5.50 STRAUMANN SCREW-RETAINED NC/RC BEGO MULTI-PLUS*	33.335.676.01-2	1.8	35	1	6.7	0.9	3	50
	33.435.676.01-2	1.8	35	1	6.7	0.9	4	50
	33.635.676.01-2	1.8	35	1	6.7	0.9	6	50
*KLOCKNER ESSENTIAL CONE 4.5 DIRECTO IMPLANTE KLOCKNER ESSENTIAL CONE 4.5 OCTACONE 12° KLOCKNER ESSENTIAL CONE 4.5 OCTACONE 25° KLOCKNER VEGA RV XIVE S 3.8 XIVE S 4.5 BIOHORIZONS 3.0 STRAUMANN SYNOCTA 6.5 STRAUMANN BLX RB STRAUMANN BLX WB STRAUMANN TLX NT STRAUMANN TLX RT STRAUMANN TLX WT DENTIUM MU SUPERLINE*	33.345.856.01-2	1.8	45	1	8.5	0.9	3	50
	33.445.856.01-2	1.8	45	1	8.5	0.9	4	50
	33.645.856.01-2	1.8	45	1	8.5	0.9	6	50

# DYNAMIC MILLING TOOL SPECIFICATIONS

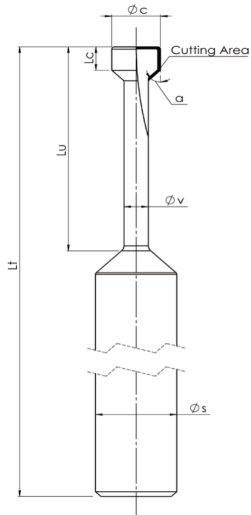

3 FLUTE T-SLOT CUTTER



MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		φc		Lc	Lu	φv	φs	Lt
"MIS C1 RP PALTOP UNIVERSAL MULTI UNIT MIS C1 WP S&M PREMIUM KHONO 3.3 S&M PREMIUM KHONO 3.8 S&M OUTLINK 3.3 S&M OUTLINK 4.1 S&M PREMIUM KHONO 4.25 BREDENT SKY NP BREDENT SKY RP ADIN TOUAREG/CLOSEFIT NP ADIN TOUAREG/CLOSEFIT UNP CAMLOG CONELOG 3.3 GLOBAL D (TEKKA) EASY IMPLANT MINI ROOT R"	33.360.756.01-2	1.8	60	1	7.5	0.9	3	50
	33.460.756.01-2	1.8	60	1	7.5	0.9	4	50
	33.660.756.01-2	1.8	60	1	7.5	0.9	6	50
"ZIMMER SCREW-VENT 3.5 ZIMMER SCREW-VENT 4.5 ASTRA EVOLUTION UNIT ABUTMENT ZIMMER TYPE 5.7 OXY FIXO	33.370.716.01-2	1.8	70	1	7.1	0.9	3	50
	33.470.716.01-2	1.8	70	1	7.1	0.9	4	50
	33.670.716.01-2	1.8	70	1	7.1	0.9	6	50
"NOBEL BIOCARE BRANEMARK RP NOBEL BIOCARE MULTI-UNIT RP BIOMET 3i OSSEOTITE NP BTI EXTERNAL CONNECTION NP BTI INTERNAL CONNECTION RP MIS MULTI-UNIT ST KEYSTONE PRIMA NP KEYSTONE PRIMA RP KEYSTONE PRIMA WP NEOSS PROACTIVE 3.4 NEOSS PROACTIVE 4.1 BIOMET 3i OSSEOTITE WP BTI EXTERNAL CONNECTION WP BTI MULTI-IM UNIVERSAL RP ANTHOGYRD MULTI-UNIT 4.8 BEGO MINI BTI INTERNAL WP LASAK MULTI-UNIT ON/OR SIC SICACE 3.3 SIC SICACE 4.2 IMPLANT DIRECT"	33.390.716.01-2	1.8	90	1	7.1	0.9	3	50
	33.490.716.01-2	1.8	90	1	7.1	0.9	4	50
	33.690.716.01-2	1.8	90	1	7.1	0.9	6	50
"STRAUMANN INTERNAL OCTAGON RP STRAUMANN INTERNAL OCTAGON 6.5"	33.315.708.01-2	1.8	15	1	7	1	3	50
	33.415.708.01-2	2	15	1	7	1	4	50
	33.615.708.01-2	2	15	1	7	1	6	50
STRAUMANN SYNOCTA RP	33.330.708.01-2	2	30	1	7	1	3	50
	33.430.708.01-2	2	30	1	7	1	4	50
	33.630.708.01-2	2	30	1	7	1	6	50
"NOBEL BIOCARE ACTIVE RP NOBEL BIOCARE ACTIVE WP"	33.335.758.01-2	2	35	1	7.5	1	3	50
	33.435.758.01-2	2	35	1	7.5	1	4	50
	33.635.758.01-2	2	35	1	7.5	1	6	50
"OSSTEM TS RP CAMLOG SCREW-LINE 5.0 CAMLOG SCREW-LINE 6.0"	33.345.808.01-2	2	45	1	8	1	3	50
	33.445.808.01-2	2	45	1	8	1	4	50
	33.645.808.01-2	2	45	1	8	1	6	50
"NOBEL BIOCARE REPLACE RP ASTRA LILAC NOBEL BIOCARE REPLACE WP ASTRA EVOLUTION 4.8 NOBEL BIOCARE BRANEMARK WP ASTRA EVOLUTION 5.4 NOBEL BIOCARE REPLACE 6.0"	33.390.958.01-2	2	90	1	9.5	1	3	50
	33.490.958.01-2	2	90	1	9.5	1	4	50
	33.690.958.01-2	2	90	1	9.5	1	6	50

## SCREWDRIVER ADAPTOR

### Screwdriver for the Dynamic Scanbody System



Ref. 43.621.410.01-2  
Screwdriver with manual handle  
Standard length: 21 mm



Ref. 43.621.415.01-2  
Tiny Screwdriver with manual handle  
Length: 21 mm



Ref. 43.624.410.01-2  
Contra-angle  
Length: 24 mm



Ref. 43.620.411.01-2  
Multi-Unit  
Contra-angle  
Length: 20 mm

## COMPLEMENTS



### Manual handle

Made of stainless steel.  
They are used to connect screwdriver bits with the contra-angle connection

### Large manual handle for laboratory

Ref. 49.601.000.03-2

Ideal to manipulate models in the laboratory  
Length: 55.65 mm



### Manual handle for clinic

Ref. 49.601.000.01-2

Clinic handle: used to position the prosthesis in the mouth prior to torque control in the clinic.  
Length: 15.65 mm



### Universal manual torque wrench prosthetic

Ref. 11.990.990.07-2

Torque wrench  
4 mm square connection.  
Torque 10-35N.c



### Dynamic Screw Transfer

Ref. 49.413.000.01-2

### Manual torque wrench adapter prosthetic

Piece to connect the screwdriver with contra-angle connection to the torque wrench.



Universal Manual torque wrench adapter

Ref. 49.604.000.05-2

4 mm Square connection



Straumann Manual torque wrench adapter

Ref. 49.604.000.07-2

Straumann connection



Nobel Biocare Manual torque wrench adapter

Ref. 49.604.000.08-2



MIS Manual torque wrench adapter

Ref. 49.604.000.09-2

## DYNAMIC SCREWDRIVERS

Screwdriver with hexalobular head, exclusively to the 3.0 Dynamic Abutment System.  
Lengths: 18, 24, 32 mm



Ref. 43.618.201.01-2  
Hexalobular 1,70 mm.  
Length: 18 mm



Ref. 43.632.201.01-2  
Hexalobular 1,70 mm.  
Length: 32 mm



Ref. 43.624.201.01-2  
Hexalobular 1,70 mm.  
Length: 24 mm

## DAS MU SYSTEM COMPONENTS



MU Dynamic TiBase  
Non-engaging\*  
31.322.209.01-2

Engaging\*  
31.312.209.01-2



MU Dynamic 3TiBase  
Non-engaging\*  
31.322.209.21-2



Reference Scanbody  
Non-engaging\*  
54.322.209.31-2



Engaging\*  
54.312.209.31-2



Healing Cap  
Regular  
40.320.003.88-2



Wide  
40.320.003.89-2



MU ScAnalog  
23.412.209.01-2



MU Scanbody 4,5 mm  
53.412.209.01-2



MU Scanbody 8 mm  
Non-engaging\*  
53.422.209.02-2



MU Dynamic Scanbody  
52.408.137.01-2



Dynamic Scanbody Adaptor  
50.312.209.01-2



Screwdriver Adaptor  
43.621.410.01-2



43.624.410.01-2



Impression coping  
Non-engaging\*  
29.301.000.11-2



Titanium Abutment  
Non-engaging\*  
35.312.209.21-2

Engaging\*  
35.322.209.21-2



Digital Analog  
34.312.209.01-2



Analog  
22.612.209.01-2



Digital Analog Positioner  
49.309.000.01-2



Dynamic Screw  
41.320.040.01-2



Provisional (temporary)  
Dynamic Screw  
41.320.050.02-2



Straight Screw  
40.320.003.06-2

COMPONENTS OPTIONS: \* Non-engaging + R \* Engaging + NR

## DAS MU SYSTEM COMPONENTS

### Peek Pins

#### Type A

49.414.000.01-2 (6 mm)  
49.415.000.01-2 (9 mm)  
49.416.000.01-2 (13 mm)

#### Type B

49.414.000.02-2 (6 mm)  
49.415.000.02-2 (9 mm)  
49.416.000.02-2 (13 mm)

#### Type C

49.414.000.03-2 (6 mm)  
49.415.000.03-2 (9 mm)  
49.416.000.03-2 (13 mm)

#### Type D

49.416.000.04-2 (13 mm)

#### Type E

49.416.000.05-2 (13 mm)


### CAPS

#### Regular

49.418.000.01-2 (3,8 mm)  
49.419.000.01-2 (6 mm)  
49.420.000.01-2 (8 mm)

#### Wide

49.418.000.02-2 (3,8 mm)  
49.419.000.02-2 (6 mm)  
49.420.000.02-2 (8 mm)



### Ratchet

49.409.000.01-2



### Screwdriver

43.321.316.01-2



43.322.316.01-2



### Mu ANG Insertion tool

49.422.000.01-2



### Dynamic Screwdriver

43.618.201.01-2 (18 mm)  
43.624.201.01-2 (24 mm)  
43.632.201.01-2 (32 mm)



### Screwdriver Hex.1,2

43.601.103.02-2



### MU DMTone

33.390.716.01-2 Shank Ø3  
33.490.716.01-2 Shank Ø4  
33.690.716.01-2 Shank Ø6

# INTERNAL DAS MU SYSTEM COMPONENTS



**MU Dynamic TiBase**  
Type A Engaging\*  
31.312.210.01-2



**Dynamic Screw**  
41.318.050.01-2




**Type B Engaging\***  
31.313.210.01-2



**Provisional (temporary) Dynamic Screw**  
41.318.057.01-2



**Non-engaging\***  
31.322.210.01-2



**Ratchet**  
49.409.000.02-2



**Reference Scanbody Engaging\***  
54.312.210.31-2



**Screwdriver**  
43.321.320.01-2




**Healing Cap Regular**  
40.318.003.89-2




**Digital Analog**  
34.312.210.01-2




**Digital Analog Positioner**  
49.309.000.01-2



**Peek Pins**  
Type A  
49.414.000.01-2 (6 mm)  
49.415.000.01-2 (9 mm)  
49.416.000.01-2 (13 mm)



Type B  
49.414.000.02-2 (6 mm)  
49.415.000.02-2 (9 mm)  
49.416.000.02-2 (13 mm)



Type C  
49.414.000.03-2 (6 mm)  
49.415.000.03-2 (9 mm)  
49.416.000.03-2 (13 mm)



Type D  
49.416.000.04-2 (13 mm)



Type E  
49.416.000.05-2 (13 mm)



**Dynamic Screwdriver**  
43.618.201.01-2 (18 mm)  
43.624.201.01-2 (24 mm)  
43.632.201.01-2 (32 mm)



**MU DMTone**  
33.390.716.01-2 Shank Ø3  
33.490.716.01-2 Shank Ø4  
33.690.716.01-2 Shank Ø6



**CAPS Regular**  
49.418.000.01-2 (3,8 mm)  
49.419.000.01-2 (6 mm)  
49.420.000.01-2 (8 mm)



**Wide**  
49.418.000.02-2 (3,8 mm)  
49.419.000.02-2 (6 mm)  
49.420.000.02-2 (8 mm)

COMPONENTS OPTIONS: \* Non-engaging - R \* Engaging - NR

## TERMS AND CONDITIONS

These guarantee terms and conditions ("T&C") cover the entire range of Talladium products ("Products"), manufactured by TALLADIUM ESPAÑA S.L. and distributed by Geoda Medical S.L. or official dealers. The guarantee described in these T&C is exclusively in benefit of the clinician ("Clinician") and of the dental technician ("Technician") and not for the benefit of third parties or institutions, including patients.

## GUARANTEE PERIOD

TALLADIUM ESPAÑA S.L. offers a lifelong guarantee for its entire range of products starting from the date of issue of the invoice.

## GUARANTEE SCOPE

Subject to the limitations and exceptions described in these T&C, TALLADIUM ESPAÑA S.L. will offer the following benefits:

**QUALITY:** If there are defects in the materials or in the manufacturing of the Product, TALLADIUM ESPAÑA S.L. will replace the Product with no additional cost.

**SAFETY:** If, having complied with all the product indications, the prosthesis should have to be made again, due to a fault in the Dynamic Abutment or Dynamic Titanium Base system, TALLADIUM ESPAÑA S.L. will replace the abutments and screws necessary to remake the prosthesis, as well as the costs derived from its manufacturing.

In case of having used our products and having complied with all the product indications, the implants suffer any damage, TALLADIUM ESPAÑA S.L. will pay the cost of the implants. This coverage will only be valid during the first 6 months after the collocation of the prosthesis which includes our products.

## CLAIM REQUIREMENTS AND PROCEDURE

To receive the benefits indicated in these T&C, the treating Clinician must satisfy the following requirements:

- The claim must be notified to TALLADIUM ESPAÑA S.L. within (30) days since the date the claimed defect was detected.
- This requires that the Clinician or Technician must contact the customer service department by telephone or by e-mail to make the claim.
- A claim form will be completed, which, together with a document or report which justifies the faulty Product and the faulty Product itself, will be sent by the customer to TALLADIUM ESPAÑA S.L. offices, within the previously indicated period.
- Clinicians or Technicians presenting a claim in agreement with these T&C must be up to date in any payments owing to TALLADIUM ESPAÑA S.L. or to any of its subsidiaries, at the time when the claim form is presented.
- All the use procedures of our Products must be carried out in agreement with the instructions of TALLADIUM ESPAÑA S.L. as well as in accordance with commonly accepted dentistry practices.
- The expenses derived from this procedure will be assumed by the customer. The return shipping costs will be assumed by TALLADIUM ESPAÑA S.L. in all those cases covered by these T&C.

Regardless of the guarantee rights, claims should be notified as soon as possible in order to comply with regulatory requirements.

## GENERAL LIMITATIONS OF THIS GUARANTEE

With the exception of the guarantee described in these T&C, neither TALLADIUM ESPAÑA S.L. nor its representatives, nor third parties manufacturing or distributing the Products, represent or offer a guarantee, agreement or any other express or implicit, oral or written, commitment, with respect to the Products (without limitation), including guarantees involved in the marketing, durability or suitability for individual uses or purposes. In addition and within the maximum extent permitted by the relative law, TALLADIUM ESPAÑA S.L. rejects (on its own behalf, and on behalf of its representatives and third parties that manufacture or distribute Products) any responsibility with respect to any direct or indirect damage caused, which may result from or be a consequence of the design, composition of the dental prosthesis into which the Products are integrated.


## GUARANTEE EXCLUSIONS

TALLADIUM ESPAÑA S.L. limits this guarantee to:

- Transformed abutments that form part of the dental prosthesis. But not the screws used to anchor them.
- Those products that are not used with the accessories and parts marketed by Talladium España

## AMENDMENT OR SUSPENSION OF THE GUARANTEE

TALLADIUM ESPAÑA S.L. reserves the right to amend or withdraw these T&C at any time and without prior notification. Any modification or suspension shall not affect products already placed in patients.




This printed version is probably outdated and may not include all products or compatibilities.

**Scan and download the latest version of this catalogue**

[www.dynamicabutment.com](http://www.dynamicabutment.com)



[www.dynamicabutment.com](http://www.dynamicabutment.com)

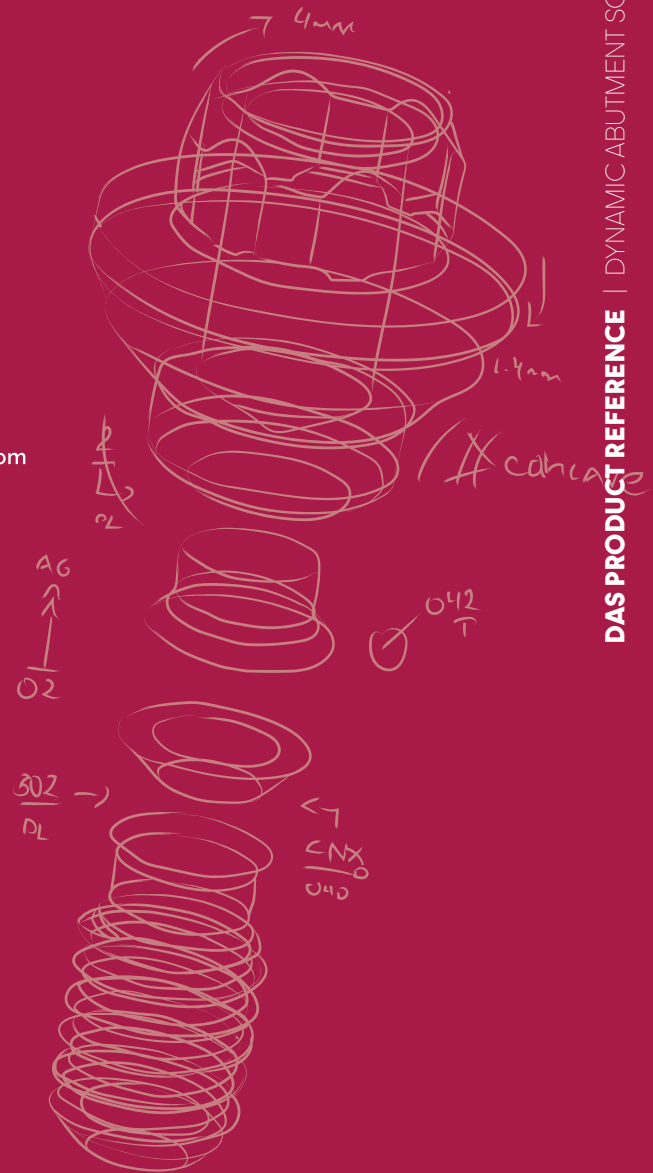

Virginia Woolf, 17  
25005 · Lleida (Spain)

INTERNATIONAL +34 873 450 709  
das@dynamicabutment.com

SPAIN +34 973 289 580  
spain@dynamicabutment.com